

eclipse
WITH
autoSAT®

Eclipse 5™ with autoSAT®

Oxygen Concentrator

TECHNICAL SERVICE MANUAL




CAIRE®

TABLE OF CONTENTS

| | | | |
|---|-----------|--|-----------|
| General Information | 4 | Power Cartridge | 19 |
| Warning and Caution Statements | 4 | Typical New Power Cartridge Operation Time | 20 |
| Introduction to the Eclipse 5 Oxygen System ... | 6 | Charging Algorithm..... | 22 |
| Eclipse 5 Oxygen System Specifications | 7 | Training The Patient | 23 |
| Pulse Dose Mode Specifications | 8 | Introduction | 23 |
| Power Accessory Specifications | 8 | Pre-Delivery Check List..... | 23 |
| AC Power Supply | 8 | Indications for Use | 24 |
| DC Power Supply..... | 8 | Contraindications | 24 |
| Power Cartridge (Battery) | 8 | Basic Concept Training | 24 |
| Independent Safety Testing | 9 | Safety Guidelines and Operational Safety Warnings/Caution..... | 24 |
| Electromagnetic Compatibility | 10 | Locating the Eclipse 5 for Proper Use and Ventilation | 25 |
| Guidance and Manufacturer’s Declarations.... | 10 | The Users Manual..... | 25 |
| How The Eclipse 5 Works | 12 | Showing Panel Buttons, Indicators, Alerts and Alarms..... | 25 |
| Introduction..... | 12 | Showing Power Cartridge Power Level | 26 |
| ATF® Concentrator Module..... | 12 | Selecting the Proper Flow Mode and Setting .. | 26 |
| Compressor and Compressor Enclosure..... | 13 | Selecting Continuous Flow Mode..... | 26 |
| Power Distribution..... | 13 | Selecting Pulse Dose Mode | 26 |
| Control Board | 13 | “Power Cartridge (Battery) Conservation” Feature | 27 |
| Control Panel..... | 14 | Adjusting the Pulse Mode Sensitivity Setting .. | 27 |
| User Controls & System Status Indicators..... | 14 | Adjusting Rise Time | 28 |
| Continuous Flow Mode | 15 | Connecting the AC Power Supply | 28 |
| Pulse Dose Mode | 15 | Connecting the DC Power Supply | 29 |
| Provider Mode Functions..... | 16 | Active Lifestyle Training..... | 29 |
| Alarm Code..... | 16 | Attach the Universal Cart | 30 |
| Pulse Mode Sensitivity Adjustment..... | 16 | Using Around the House | 30 |
| Hours of Operation | 16 | Traveling by Vehicle | 30 |
| 9V Battery Status..... | 16 | Traveling by Air | 32 |
| Rise Time (Bolus Delivery) | 16 | Traveling by Cruise Ship | 32 |
| Software Version | 16 | Traveling by Train..... | 32 |
| Service Mode Functions | 17 | Eclipse 5 Maintenance | 33 |
| Eclipse 5 Data Acquisition Tool (EDAT) | 17 | Weekly Maintenance—Patient | 33 |
| Power Supplies..... | 18 | Clean the Air Inlet Filter | 33 |
| AC Power Supply | 18 | Clean and Care for the Tubing and Cannula .. | 33 |
| DC Power Supply..... | 18 | | |

TABLE OF CONTENTS (CONTINUED)

| | | |
|---|-----------|--|
| Clean the Cabinet and Control Panel and Power Supplies..... | 33 | Troubleshooting, Service, and Repair Procedures53 System Troubleshooting and Alarms..... 54 Alarm Conditions and Alarm Codes 57 Malfunction Codes 59 System Schematics and Diagrams 60 Oxygen Circuit 62 Remove and Replace the ATF Module..... 62 Remove and Replace the Product Tank Assembly (PN 4378-SEQ) Eclipse 5 66 Electronics 69 Remove and Replace the Control Board Assembly 69 Remove and Replace the Buzzer Wire Harness 71 Control Board Connector Diagram 72 Remove and Replace the Power Manager Printed Circuit Board 73 Compressor 77 Remove and Replace the Compressor Box 77 Maintenance and Replacement Parts 81 Preventative Maintenance Parts 81 Replacement Parts List 81 Optional Accessories 82 |
| Monthly Maintenance—Patient | 34 | |
| Care for the Power Cartridge..... | 34 | |
| Calibrating the Power Cartridge | 34 | |
| Patient Training Checklist | 35 | |
| Annual Maintenance—Provider | 36 | |
| Introduction | 36 | |
| Annual Maintenance Check List | 36 | |
| Checking and Replacing the Power Cartridge | 36 | |
| Eclipse 5 Monthly Run-Time Cycle..... | 36 | |
| Annual Maintenance Procedures | 37 | |
| Removing the Unit Cover | 37 | |
| Remove and Replace 9 Volt Battery | 41 | |
| Remove and Replace HEPA Filter..... | 42 | |
| Internal Filters | 42 | |
| Remove and Replace the Compressor Intake Filter..... | 44 | |
| Reinstalling or Replacing the Unit Cover..... | 46 | |
| Test Procedures | 47 | |
| Purity and Flow Rate Test Procedure - Preferred Method | 47 | |
| Purity and Flow Rate Test Procedure- Alternate Method | 47 | |
| Assembly and Alarm Verification Tests | 48 | |
| Record Hours of Operation & Software Version | 49 | |
| Electrical Safety Test | 50 | |
| Cleaning the Eclipse 5..... | 50 | |
| Provider Service and Maintenance Record..... | 51 | |
| Shipping and Transporting the Eclipse 5 | 52 | |
| Storing the Eclipse 5 | 52 | |
| Discarding | 52 | |

| | |
|--|-----------|
| CAIRE Inc. Customer Service Contact Information | 83 |
|--|-----------|



GENERAL INFORMATION

This technical manual will familiarize you with Provider-specific information regarding the Eclipse 5 Oxygen System. Instructions in this manual are intended to help ensure that:

- Providers are familiar with Eclipse 5 system components and system principles of operation
- Providers are given proper guidance in the use of the Eclipse 5 and its accessories that can be conveyed to patients
- Providers are made aware of the care, diagnostics, maintenance, and repair of the Eclipse 5

Warning and Caution Statements

Safety instructions are defined as follows:

| | | |
|----------|--|--|
| WARNING: |  | Important safety information for hazards that might cause serious injury. |
| | | |
| CAUTION |  | Important information for preventing damage to the Eclipse 5. |
| | | |
| NOTE: | | Places emphasis on an operating characteristic or important consideration. |

| Internal Symbols | |
|---|--|
| | External Power Indicator |
| | Power Cartridge (battery) Status Gauge |
| | Power Cartridge Symbol |
| A | Amperes |
| O₂ | Oxygen Output |
| | Recycle Symbol |
| | FAA Approved Symbol: The U.S. Federal Aviation Administration (FAA) has approved this device for use on-board commercial aircraft. |
| | Flow Setting Indicator |
| | Pulse Mode Operation |
| | Device operating normally; power button |
| | Increase Flow Setting |
| | Decrease Flow Setting |
| ISO 7000; Graphical symbols for use on equipment—Index and synopsis | |
| | Storage temperature limitation range is -4°F to 140°F (-20°C to 60°C). Reg. # 0632 |
| | Portable humidity range is 15 to 95%. Base humidity range is 30 to 75%. Reg. # 2620 |
| | Atmospheric pressure limitation. Reg. # 2621 |
| | Operator's manual; operating instructions. Reg. # 1641 |
| | Name and address of manufacturer. Reg. # 3082 |
| | Date of manufacturer. Reg. # 2497 |
| REF | Catalog Number. Reg. # 2493 |
| SN | Serial Number. Reg. # 2498 |
| | This way up. Reg. # 0623 |
| | Fragile, handle with care. Reg. # 0621 |
| | Keep away from rain, keep dry. Reg. # 0626 |

| | Stacking limit by number. Reg. # 2403 |
|--|---|
| ISO 7010: Graphical symbols—Safety colors and safety signs—Registered safety signs | |
| | The instruction manual must be read. Reg. # M002 |
| | Keep away from open flame, fire, sparks. Open ignition source and smoking prohibited. Reg. # P003 |
| | Do not smoke near unit or while operating unit. Reg. # P002 |
| Council Directive 93/42/EEC; concerning medical devices | |
| EC REP | Authorized representative in the European Community |
| CE 0459 | This device complies with the requirements of Directive 93/42/EEC concerning medical devices. It bears the CE marking as shown. |
| IEC 60417 | |
| | Class II Equipment, Double Insulated Reg. # 5172 |
| | Alternating Current Reg. # 5032 |
| | Direct Current Reg. # 5031 |
| | Type BF applied part (degree of protection against electric shock). Reg. # 5333 |
| CSA Certification | |
| | Certified for both the U.S. and Canadian markets, to the applicable U.S. and Canadian standards. |
| Contains FCC ID: WAP2001 FCC Notice | |
| 21 CFR 801.15: Code of Federal Regulations Title 21 | |
| RX ONLY | Federal law restricts this device to sale by or on the order of a physician. |
| Council Directive 2012/19/EU: waste electrical and electronic equipment (WEEE) | |
| | WEEE |
| IEC 60601-1: Medical electrical equipment Part 1 General requirements for basic safety and essential performance | |

| IP22 | Drip Proof Equipment - IP22: The Eclipse 5 and the AC power supply provide protection against the harmful effects of ingress of liquids (IP22 per IEC 60529) |
|---------------|--|
| IEC 60601-1-8 | |
| | Low Priority Technical Alarm |

FCC NOTICE:

This device may contain CYBLE-022001-00, including the antenna 2450AT18B100 from Johnson Technology, complies with par 15 of the FCC rules. The device meets the requirements for modular transmitter approval as detailed in FCC public Notice DA00-1407. Transmitter operation is subject to the following two conditions (1) This device may not cause harmful interference, and (2) This device must accept any interference received, including interference that may cause undesired operation.

This product may be covered by one or more patents, US and international. Please visit our website below for the listing of applicable patents. Pat.: patents.gtls.io.

Aircraft Use:

CAIRE confirms that this machine meets the Federal Aviation Administration (FAA) requirements (RTCA/DO-160, section 21, category M) for all phases of air travel.

| Wireless Technology | |
|--|------------------|
| Technology used | Bluetooth |
| Connection types | SSP, iAP2, GATT |
| Frequency | 2402 to 2480 MHz |
| Max RF power output | +4 dBm |
| Operating range | 10m (Class 2) |
| It is recommended that the machine is at a minimum distance of 0.43" (1.1 cm) from the body during operation. Not applicable to masks, air tubing, or accessories. | |

INTRODUCTION TO THE ECLIPSE 5 OXYGEN SYSTEM

ECLIPSE 5



UNIVERSAL CART



PN: 5991-SEQ



AC POWER SUPPLY WITH NEMA POWER CORD



PN: 5941-SEQ (three LED model)



PN: 20852326S (with IEC type A cord), 20852325S (with IEC type C cord), and 20852324S (with IEC type G cord) (two LED model)

DC POWER SUPPLY




PN: 5942-SEQ

POWER CARTRIDGE (BATTERY)



PN: 7082-SEQ

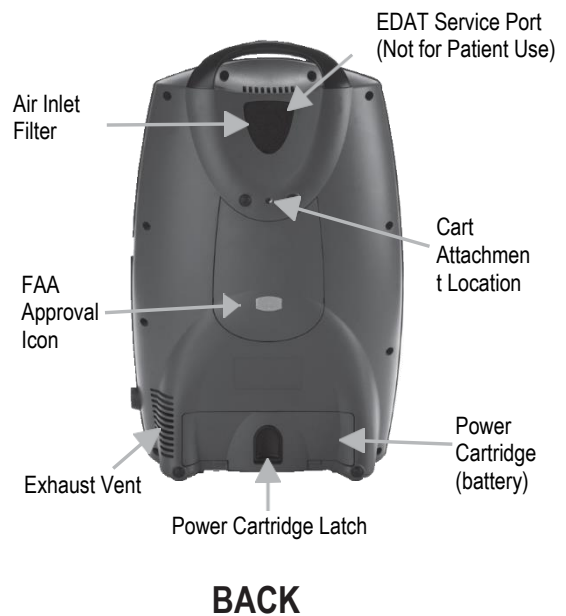

ECLIPSE 5 OXYGEN SYSTEM SPECIFICATIONS

Oxygen Concentrator

| | |
|---|---|
| Dimensions (H x W X D) | 19.3 x 12.3 x 7.1 inches (49.0cm x 31.2cm x 18.0cm) |
| Weight Eclipse 5 Power Cartridge | 15.0 pounds 3.4 pounds |
| Flow Settings Continuous Flow (measured in Liters Per Minute LPM) Pulse Dose (measured in mL) | 0.5 to 3.0 LPM (0.5 liter increments) Settings 1.0-6.0: 16mL, 24mL, 32mL, 40mL, 48mL, 56mL, 64mL, 72mL, 80mL, 88mL, 96mL Settings 7-9: 128mL, 160mL, 192mL |
| Continuous Flow Accuracy | +/- 10% or 200ml/min, whichever is greater |
| Oxygen Concentration | 87–95.5% for all flow settings |
| Maximum System Pressure | 14 psig (96.5 kPa) |
| Oxygen Output Pressure | 5.0 psig (34.5 kPa) nominal |
| Oxygen Concentration Status Indicator | Green Light = Normal Operation Yellow Light = Warning or Caution, less than 85% ± 3% Red Light Flashing = Abnormal Operation, less than 70% ± 5% (Note: only for 3-LED models) |
| Nominal Sound Level 3.0 LPM Continuous Flow 3.0 Pulse Dose Mode | 48 dB(A) 40 dB(A) Less than 57 dB while alarming |
| Operating Environment Temperature Humidity | 50° F to 104° F (+10° to 40°C) 10% to 95%, Non-condensing, 82.4°F (28°C) Maximum Dew point |
| Storage Environment Temperature Humidity | -4° F to 140° F (-20° to 60°C) Up to 95% Non-condensing |
| Altitude | 0 – 13,123 feet (0 - 4,000 meters) |
| Nominal Power 0.5 LPM Continuous flow 3 LPM Continuous Flow 1.0 Pulse Dose Setting 6.0 Pulse Dose Setting Battery Charging | 48 Watts 145 Watts 45 Watts 95 Watts 50 Watts |
| Nominal Power Cartridge operating time* Continuous Flow 2.0 LPM 3.0 LPM Pulse Dose (@ 12 BPM) Setting 2.0 Setting 6.0 | 2.0 hours 1.3 hours 5.2 hours 3.5 hours * Note: Times will <u>decrease</u> with higher bolus size, breath rate, ambient temperature, power cartridge age and use over time. |
| Outlet Pressure | Nominal: 7.0 psig Maximum: 14.0 psig |
| Continuous Flow Indication | Expressed in liters per minute (LPM) |
| Audible Alarm Indicators | <ul style="list-style-type: none"> • Loss of Power/Hot Power Cartridge • Low Power Cartridge/Warm Power Cartridge • Low Oxygen Output • O₂ Flow Outside Normal Limits • Unit Malfunction • Low 9V battery (Note: only for 3-LED model) |

| | |
|-----------------------|---|
| Back-Up Alarm Power | 9V Internal Battery |
| Filters | Air Inlet, HEPA, Compressor Intake |
| Device Classification | IEC Class I, Type B Applied Part, IP0 (3 LED model) IEC Class II, Type BF Applied Part, IP22 (2 LED model) |

Pulse Dose Mode Specifications

| | |
|------------------------------|--|
| Pulse Settings | 1.0 to 6.0: 16mL, 24mL, 32mL, 40mL, 48mL, 56mL, 64mL, 72mL, 80mL, 88mL, 96mL; 7-9: 128mL, 160mL, 192mL |
| Trigger Sensitivity | Adjustable between settings of 1 (most sensitive) to 3 (least sensitive) |
| Adjustable Bolus Rise Time | Adjustable settings of Fast(factory setting), Medium, or Slow |
| Trigger Criteria | <ul style="list-style-type: none"> Cannula pressure has dropped below the trigger point (typically between 0.135—0.37 cm of H₂O of negative pressure) At least 1¼ seconds has passed since the last pulse began |
| Minimum time between breaths | 1.25 seconds (max. 3 consecutive breaths) |
| Response to Missing Breaths | While in Pulse Dose Mode, the Eclipse 5 is always monitoring for breath detection. After 15 seconds of no breath detected, the Eclipse 5 “delivers” Continuous Flow at the last Continuous Flow setting. After another 15 seconds, the Eclipse 5 stops delivering Continuous Flow and waits 15 seconds for a breath. The Eclipse 5 will stay in this modality until a breath is detected. (See Power Cartridge Conservation Feature, page 26.) |

The expected service life is a minimum of 5 years.

| BOLUS VOLUME (+/- 15%) | Pulse Dose Setting | Bolus Size (± 15%) mL | AC Power Supply and Power Cartridge (Battery) | DC Power Supply |
|------------------------|--------------------|-----------------------|---|-----------------|
| | | | Max Breath Rate | Max Breath Rate |
| | 1.0 | 16 | 40 | 40 |
| | 2.0 | 32 | 40 | 40 |
| | 3.0 | 48 | 40 | 40 |
| | 4.0 | 64 | 40 | 31 |
| | 5.0 | 80 | 37 | 25 |
| | 6.0 | 96 | 31 | 20 |
| | 7 | 128 | 23 | 15 |
| | 8 | 160 | 18 | 12 |
| | 9 | 192 | 15 | 10 |

NOTE: Bolus volume decreases as breath rate exceeds published range.

Power Accessory Specifications

AC Power Supply

| | |
|----------------|----------------------|
| Input Voltage | 100-240VAC, 50-60 Hz |
| Input Power | 245-260 VA |
| Output Voltage | 28 VDC |
| Output Power | 200W |

DC Power Supply

| | |
|----------------|------------|
| Input Voltage | 11.5-16VDC |
| Output Voltage | 26 VDC |
| Output Power | 150W Max |

Power Cartridge (Battery)

| | |
|-------------------------------|--|
| Output voltage | 14.8 VDC |
| Capacity | Quantity (2) 97.5 W-hrs batteries (Each containing 7.92 grams equivalent Lithium content) |
| Nominal Power Cartridge Life | 80% Capacity after 500 Charge/Discharge cycles |
| Power Cartridge Recharge Time | 1.8 to 5.0 hours, dependent on flow setting, to achieve 80% capacity from a fully discharged Power Cartridge |

Independent Safety Testing

| | |
|---|--|
| Eclipse System and Eclipse Concentrator | |
| Safety | IEC 60601-1 :1988 + A1 :1991 + A2 :1995 + Corrigendum (6/95) EN 60601-1(1990) + A1(1993) + A2(1995) + A12(1993) + A13(1996) + Corrigenda (7/94) |
| Electromagnetic Compatibility | FCC 15B (Sec. 107 & 109), EN55011, EN60601-1-2 :2014 and EN 60601-1-2:2015: ETSI EN 301 489-1 V2.1.1 and ETSI EN 301489-17 V3.1.1 (2017-02); EN6100-3-2, EN61000-3-3, IEC61000-4-2, IEC61000- 4-3, IEC61000-4-4, IEC61000-4-5, IEC61000-4-6, IEC61000-4-8, IEC61000-4-11, IEC 60601-1-2 :2001, RTCA DO 160 Rev G |
| AC Power Supply (3 LED model, Model 5941) | |
| Safety | IEC 60601-1:1988 + A1:1991 + A2:1995 |
| Electromagnetic Compatibility | FCC 15B (Sec. 107 & 109), EN55011, EN60601-1-2 :2001, EN6100-3-2, EN61000-3-3, IEC61000-4-2, IEC61000-4-3, IEC61000-4-4, IEC61000-4-5, IEC61000-4-6, IEC61000-4-8, IEC61000-4-11, EN55014-1 |
| AC Power Supply (2 LED model) | |
| Safety | IEC60601-1, 3rd Edition, ANSI / AAMI ES60601-1, CSA 22.2 No. 60601-1, EN60601-1, 3rd Edition, CE Mark (LVD) |
| Electromagnetic Compatibility | Emissions: EN55011, FCC Part J15, Class B, Conducted, EN55011, FCC Part J15, Class B, Radiated EN61000-3-2, EN61000-3-3, EN61000-4-2, EN61000-4-3, EN61000-4-4, EN61000-4-5, EN61000-4-6, EN61000-4-11 |
| DC Power Supply, Model 5942 | |
| Safety | Portions of IEC 60601-1:1988 + A1:1991 + A2:1995 |
| Electromagnetic Compatibility | FCC 15B (Sec. 107 & 109), EN55011, EN60601-1-2 :2014 and EN 60601-1-2:2015: ETSI EN 301 489-1 V2.1.1 and ETSI EN 301489-17 V3.1.1 (2017-02); EN6100-3-2, EN61000-3-3, IEC61000-4-2, IEC61000- 4-3, IEC61000-4-4, IEC61000-4-5, IEC61000-4-6, IEC61000-4-8, IEC61000-4-11, IEC 60601-1-2 :2001, RTCA DO 160 Rev G |
| Power Cartridge 2400, PN 7082 | |
| Safety | IEC 62133:2013 and IEC 62133 (edit), UL60950-1, First Edition (UL File MH29443), IEC 60601-1:1988 + A1:1991 + A2:1995, UN Transportation Tests T1-T8 |
| Electromagnetic Compatibility | FCC 15B (Sec. 107 & 109), EN55011, EN60601-1-2 :2014 and EN 60601-1-2:2015: ETSI EN 301 489-1 V2.1.1 and ETSI EN 301489-17 V3.1.1 (2017-02); EN6100-3-2, EN61000-3-3, IEC61000-4-2, IEC61000- 4-3, IEC61000-4-4, IEC61000-4-5, IEC61000-4-6, IEC61000-4-8, IEC61000-4-11, IEC 60601-1-2 :2001, RTCA DO 160 Rev G |
| Any CSA-CUS mark for the Eclipse 5 system does not encompass operation with the DC Power Supply Model 5942. | |

ELECTROMAGNETIC COMPATIBILITY

This equipment has been tested and found to comply with the limits for medical devices to the IEC60601-1-2 Electromagnetic Compatibility standard. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This equipment generates, uses, and can radiate radio frequency energy and, if not installed according to the instructions, may cause harmful interference to other devices in the vicinity. There is, however no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to other devices, which can be determined by turning the equipment off and on, the User is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving device.
- Increase the separation distance between the equipment.
- Connect the equipment into an outlet on a circuit different from that which the other device(s) are connected.
- Consult with CAIRE's Technical Support Department for help.

Medical Electrical Equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in this manual.

Portable and mobile RF communications equipment can affect Medical Electrical Equipment.

The use of Accessories, transducers, and cables other than those specified, with the exception of transducers and cables sold by the Manufacturer of this device as replacement parts for internal components, may result in increased Emissions or decreased Immunity of the Eclipse 5.

The Eclipse 5 should not be used adjacent to or stacked with other equipment and that if adjacent or stacked use is necessary, the Eclipse 5 should be observed to verify normal operation in the configuration in which it will be used.

| Guidance and Manufacturer's Declaration—Electromagnetic Emissions | | |
|---|-------------------|---|
| The Eclipse 5 is intended for use in the electromagnetic environment specified below. The customer or the user of the Eclipse 5 should assure that it is used in such an environment. | | |
| Emissions Test | Compliance | Electromagnetic Environment - Guidance |
| RF emissions CISPR 11 | Group 1 | The device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment. |
| RF emissions CISPR 11 | Class B | The device is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes. |
| Harmonic emissions IEC 61000-3-2 | Class A | |
| Voltage fluctuations/ flicker emissions IEC 61000-3-3 | Complies | |

Guidance and Manufacturer’s Declaration—Electromagnetic Immunity

The Eclipse 5 is intended for use in the electromagnetic environment specified below. The customer or the user of the Eclipse 5 should assure that it is used in such an environment.

| Immunity test | Compliance level | Electromagnetic environment – guidance |
|---|---|--|
| Electrostatic discharge (ESD) IED 61000-4-2 | ±8 kV contact ±15 kV air | Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %. |
| Electrical fast transient/burst IEC 61000-4-4 | ±2 kV | Mains power quality should be that of a typical commercial or hospital environment. |
| Surge IEC 61000-4-5 | ±1 kV ±2 kV | Mains power quality should be that of a typical commercial or hospital environment. |
| Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11 | 100V-240V | Mains power quality should be that of a typical commercial or hospital environment. If the user of the Eclipse 5 requires continued operation during power mains interruptions, it is recommended that the Eclipse 5 is powered from an uninterruptible power supply (UPS). |
| Power frequency magnetic field IEC 61000-4-8 | 30A/m | Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment. |
| Conducted RF IEC 61000-4-8 | 10 Vrms 150 kHz to 80 MHz | The Eclipse 5 complies with all applicable electromagnetic compatibility requirements (EMC) according to IEC 60601-1-2:2014, for residential, commercial and light industry environments. Portable and mobile RF communications equipment should be used no closer to any part of the machine, including cables, than the recommended 10cm separation distance. The Eclipse 5 has been designed to meet EMC standards. However, should you suspect that the machine performance (e.g. pressure or flow) is affected by other equipment, move the machine away from the possible cause of the interference. |
| Radiated RF IEC 61000-4-6 | 9 V/m to 85 V/m At frequencies, up to 5.785GHz | The Eclipse 5 complies with Part 15 of the FCC rules and industry Canada license-exempt RSS standards. Operation is subject to the following two conditions: this machine may not cause harmful interference, and this machine must accept any interference received, including interference that may cause undesired operation. FCC ID: WAP2001 |

How The Eclipse 5 Works

INTRODUCTION

The Eclipse 5, Personal Ambulatory Oxygen System with autoSAT Technology is a portable medical device used to extract oxygen from the atmosphere, concentrate it to 87–95.6% and present the oxygen to the patient. The device will operate in Continuous Flow Mode or Pulse Dose Mode. In Continuous Flow Mode the oxygen is provided at a constant flow rate between 0.5 and 3.0 LPM. In Pulse Dose Mode, oxygen is supplied in a bolus at the beginning of each inspiration, providing a selectable range setting of 16mL to 192mL.

The Eclipse 5 operates from either external power or from an internal rechargeable Power Cartridge. The system includes a “Smart” battery charger that recharges the internal Power Cartridge whenever the Eclipse 5 is connected to AC or DC power. The system monitors and controls both the power source and the Power Cartridge charger.

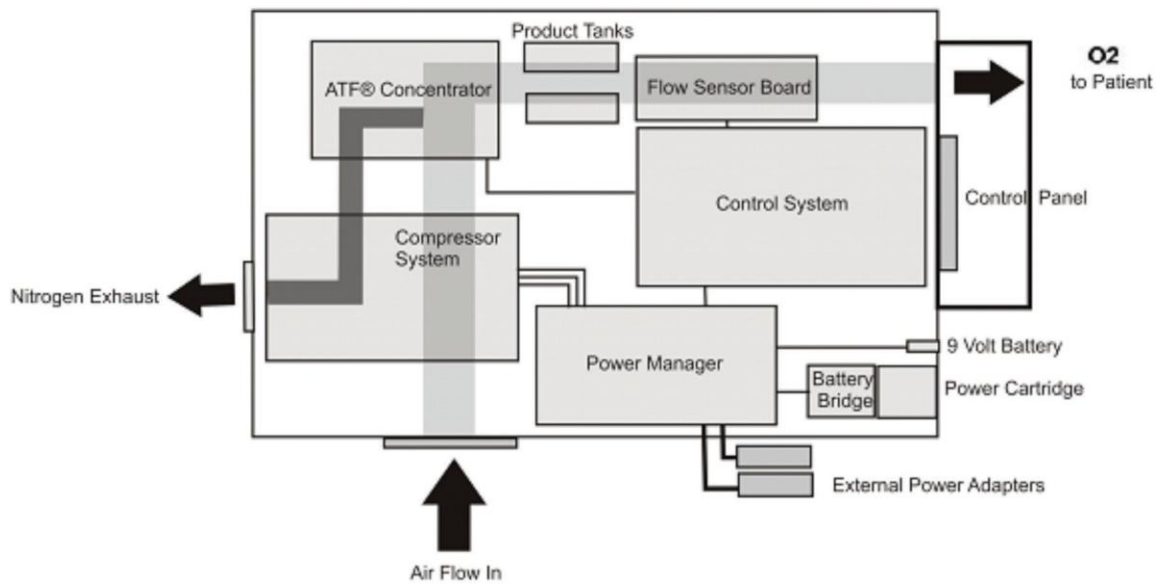


Figure 1: Eclipse 5 System Block Diagram

ATF® CONCENTRATOR MODULE

The Eclipse 5 uses a passive system to separate oxygen from air. Air flows into the Eclipse 5 where it is filtered and then enters the compressor. Pressurized air flows from the compressor into the ATF® Concentrator Module where it is separated into oxygen and nitrogen components. The air separation process uses a rotary valve system to force air through a series of pressurized sieve beds. Through a process known as “vacuum pressure swing adsorption,” nitrogen molecules are collected on an adsorbent material allowing the concentrated oxygen to be forced through a sieve bed into the product tank. The nitrogen molecules are then purged from the adsorbent material using a vacuum pressure cycle.

Oxygen flows from the product tank through a HEPA filter and past a sensor that measures flow and concentration. A flow control valve regulates the flow of concentrated oxygen presented to the patient. The process is continuously repeated during operation.

COMPRESSOR AND COMPRESSOR ENCLOSURE

The Eclipse 5 Compressor is a two-cylinder, variable speed wobble piston compressor, driven by a highly efficient Brushless DC (BLDC) motor. When air flows into the Compressor enclosure, it passes through an air intake filter/muffler that muffles sound and filters out impurities. Using one cylinder, the compressor takes in filtered air and delivers it to the ATF Module under pressure. The second cylinder draws a vacuum on the ATF module and exhausts nitrogen rich gas to the exhaust vent.

Using a multifaceted approach, sound, heat, and vibration generated by the compressor are mitigated by the compressor enclosure. Vibration and structure-borne noise are addressed by the dual axis gimbal that supports the compressor and the tubing that connects the compressor to the ATF module. The rigid walls of the compressor enclosure and the sound adsorbing foam that lines it diminish the radiated noise. The centrifugal blower mounted within the compressor enclosure serves to efficiently draw cooling air in over the compressor cylinders while simultaneously pushing exhaust gas out of the concentrator.

POWER DISTRIBUTION

The Power Manager takes external power that comes into the Eclipse 5 from the power supplies or Power Cartridge and monitors and controls power distribution to the rest of the Eclipse 5 system. The Power Manager drives the compressor, ATF module motor, blower, and provides power to the Control Board. In addition, when the unit is connected to an external power source, the power manager monitors and controls the recharging of the Power Cartridge.

CONTROL BOARD

The Control Board is at the center of nearly all Eclipse 5 functions. The board constantly monitors dynamics such as temperatures, pressures, product flow and concentration, and user input. It determines proper compressor and ATF motor speeds needed in order to provide optimum system performance. In addition, this system supports the operation of the Control Panel and its indicators.

The Control Board utilizes a proprietary ultrasonic flow and concentration sensor and a flow control valve to accurately control the flow of oxygen in Continuous Flow and Pulse Dose Modes.

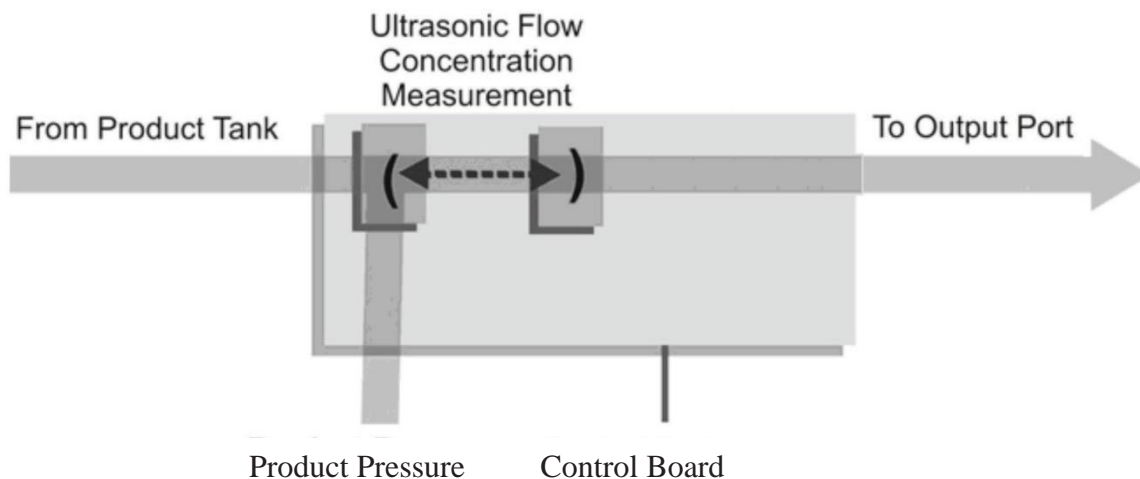


Figure 2: Flow Sensor Board Diagram

CONTROL PANEL

The control panel provides a user interface consisting of a membrane panel keyboard, Liquid Crystal Display (LCD), external power present indicator, Power Cartridge capacity indicator, alarm status indicators, and an audio transducer. The user interface informs the user of the system status and allows the user to set the desired flow rate and flow mode.



User Control Panel (3 LED model)



User Control Panel (2 LED model)



ON/OFF Button (Green) Indicator: This button powers the device ON or OFF. The Green Indicator is illuminated when the device is ON and functioning properly.



Increase or Decrease Flow Setting Buttons: Use these buttons to set the flow to your prescribed setting.



Delivery Mode Button and Indicator: The button toggles between Continuous Flow and Pulse Dose Mode. The Pulse Dose Mode activates autoSAT Technology and allows a significant increase in the operating time while powered by the battery. When the Pulse Dose Mode is activated, the green Pulse Dose Mode Indicator illuminates and a pulse of oxygen is delivered with each inspiratory effort.



ALERT (Yellow) Indicator—Low and Medium Priority Alerts: When illuminated, this indicates a low priority awareness condition or Caution. Continue to use your system and refer to the Troubleshooting Table for the proper response, or contact your Home Care Provider. A flashing yellow indicates a medium priority alert. A prompt response is necessary. (Typically low oxygen or low battery.)



ALARM (Red) Indicator—High Priority Alarms: Indicates a high priority alarm condition. An immediate response is necessary. Refer to the Troubleshooting Table and contact your home care provider. (Typically loss of power, low oxygen, or malfunction.)



Flow Setting Indicator: This is the main focus on your control panel. Your home care provider will correctly set your prescribed flow for the Continuous Flow Mode (LPM) and/or your Pulse Dose Mode (mL) settings. Each time you power the device ON, the previous mode and/or setting has been saved and will be used at start-up.



Power Cartridge (battery) Status Gauge: This indicator displays the charge remaining in the battery. Each of the five horizontal gray bars represents approximately 20% of the total battery charge. When the battery is being charged, the charge indicator bars will blink in a waterfall-type fashion. If the battery is not installed, or if it is improperly installed, the Power Cartridge (battery) Status Gauge will not be illuminated or will flash on and off.



External Power Indicator: When the Eclipse 5 is properly plugged in and is using the AC or DC Power Supply, this indicator will appear on the User Control Panel.

Buzzer: An audible alarm (or buzzer) alerts you to the operating condition of the device, either a warning or failure, and confirms a valid key press.



ON/OFF Button (Green) Indicator: This button powers the device ON or OFF. The Green Indicator is illuminated when the device is ON and functioning properly.



Increase or Decrease Flow Setting Buttons: Use these buttons to set the flow to your prescribed setting.



Delivery Mode Button and Indicator: The button toggles between Continuous Flow and Pulse Dose Mode. The Pulse Dose Mode activates autoSAT Technology and allows a significant increase in the operating time while powered by the battery. When the Pulse Dose Mode is activated, the green Pulse Dose Mode Indicator illuminates and a pulse of oxygen is delivered with each inspiratory effort.



Low Priority Technical Alarm: When illuminated, this indicates a low priority awareness condition. Continue to use your system and refer to the trouble shooting table for the proper response, or contact your Home Care Provider.



Flow Setting Indicator: This is the main focus on your control panel. Your home care provider will correctly set your prescribed flow for the Continuous Flow Mode (LPM) and/or your Pulse Dose Mode (mL) settings. Each time you power the device ON, the previous mode and/or setting has been saved and will be used at start-up.



Power Cartridge (battery) Status Gauge: This indicator displays the charge remaining in the battery. Each of the five horizontal gray bars represents approximately 20% of the total battery charge. When the battery is being charged, the charge indicator bars will blink in a waterfall-type fashion. If the battery is not installed, or if it is improperly installed, the Power Cartridge (battery) Status Gauge will not be illuminated or will flash on and off.



External Power Indicator: When the Eclipse 5 is properly plugged in and is using the AC or DC Power Supply, this indicator will appear on the User Control Panel.

Buzzer: An audible alarm (or buzzer) alerts you to the operating condition of the device, either a warning or failure, and confirms a valid key press.

CONTINUOUS FLOW MODE

Continuous Flow Mode delivers a constant flow of oxygen to a patient by means of tubing and a nasal cannula at rates between 0.5 LPM and 3.0 LPM. Within the Eclipse 5, concentrated oxygen is stored in a 500ml product tank at pressures in the range of 5 to 9 psi. This pressure gives Continuous Flow Mode the capability to deliver the indicated flow rate to the patient even if extension tubing is used, up to 50 feet long. In addition, the Eclipse 5 Continuous Flow Mode is fully compatible with humidifier use, with NC not exceeding 7 ft.

PULSE DOSE MODE

The Eclipse 5 Pulse Dose Mode delivers a measured bolus of oxygen at the very beginning of each inspiration. The approach is based on the manner in which gas is absorbed into a patient's airway. Eclipse 5 users may select pulse dose volume delivery rates. Regardless of setting, the pulse profile is a simple square-wave pulse based on a 16 mL volume. (Refer to "Pulse Profiles" table below). Pulse durations are no less than 100 milli-seconds at the beginning of the inspiration. There are three Rise Time settings (Slow, Medium, and Fast). The table below is for the FAST Rise Time setting (factory default is Fast).

| Flow Setting | Pulse Peak Flow, LPM (volumetric) | Pulse Duration (milli-second) | Bolus Volume (ml) |
|--------------|-----------------------------------|-------------------------------|-------------------|
| 1.0 | 8 | 120 | 16 |
| 2.0 | 9 | 213 | 32 |
| 3.0 | 10 | 288 | 48 |
| 4.0 | 11 | 349 | 64 |
| 5.0 | 12 | 400 | 80 |
| 6.0 | 13 | 443 | 96 |
| 7 | 15 | 512 | 128 |
| 8 | 17 | 565 | 160 |
| 9 | 19 | 606 | 192 |

Pulse Profiles

The fundamental approach to triggering and controlling the oxygen bolus in Pulse Dose Mode is as follows:

The User may select a pulse trigger sensitivity in settings ranging from 1-3. Bolus volume should be prescribed by a physician and may range from 16mL up to 192mL. The pulse will be triggered when the system meets all of the following criteria:

- The cannula pressure has dropped below the trigger point (typically between 0.135 and 0.37 cm H₂O)
- At least 1¼ seconds has passed since the last pulse began

PROVIDER MODE FUNCTIONS

Providers can access provider mode software functions using the Control Panel. All provider mode information is displayed on the LCD. The software shall advance the following Eclipse 5 **display mode** when the “No Smoking” icon is pressed:

- Alarm Code (ALRM) - Displays most recent alarm code. Additional alarm codes will also be displayed, if present, by continuing to press the + key.
- Pulse Sensitivity (PS)
- Hours of Operation (HRS)
- 9-volt Battery Status (9V)
- Rise Time (BOL)
- Control Board Software Revision (CS)
- Power Manager Software Revision (PM)

ALARM CODE

While in Continuous Flow Mode, pressing the “No Smoking” icon displays the current Eclipse 5 alarm code on the LCD. This code may be used to help diagnose conditions indicated by the alert and alarm indicators. The LCD will show “ALRM=”. Refer to the “Level 1 Maintenance” section for further information.

PULSE MODE SENSITIVITY ADJUSTMENT

During patient setup, a qualified clinician may adjust the Pulse Mode sensitivity to best suit patient inspiratory effort. The LCD will show “PS=x”. PS=1 is the most sensitive setting, PS=3 is the least sensitive setting. Factory default is PS=2.

HOURS OF OPERATION

The Eclipse 5 hour meter provides valuable information on hours of operation. Providers may display the total number of hours of operation using the Control Panel. The display counts up to “99,999”hours, then rolls over to “00000.”The LCD will show “HRS xxxxx”. Refer to the “Level 1 Maintenance” section for further information.

9-VOLT BATTERY STATUS

The status of the 9-Volt Battery is provided. This is the actual voltage of the 9-Volt battery. The LCD will show “9V=x.x”.

RISE TIME (BOLUS DELIVERY)

During patient set up, a qualified clinician may adjust the Rise Time (fast, medium or slow), i.e. how quickly the set bolus volume is delivered. The LCD will display “BOL=”. Factory default is BOL=FAST.

SOFTWARE VERSION

Providers may occasionally need to obtain the software version on the Eclipse 5 to perform maintenance. The provider may display software version numbers for both the Control Board and the Power Manager software using the Control Panel. Refer to the “Level 1 Maintenance” section for further information.

Example: CB796010: Control Board PCB: PN 7960 with Rev 1.0 software
PM796110: Power Manager PCB: PN 7961 with Rev 1.0 software

BLUETOOTH™ STATUS

OFF = off

NC = Not Connected

CNT = Connected.

SERVICE MODE FUNCTIONS

Factory maintenance or service updates may sometimes be required on the Eclipse 5. Factory and qualified factory-trained technicians can access service mode software functions by using the Service Port located on the back of the unit. The Service Port is not for patient use.



Figure 4: Eclipse 5 Service Port

ECLIPSE 5 DATA ACQUISITION TOOL (EDAT)

EDAT is the world's first computer-based data retrieval service tool for oxygen concentrators. EDAT is proprietary to CAIRE Inc., and is comprised of both hardware and software components. EDAT is CAIRE Inc.'s global solution for your service and support needs.

EDAT software is capable of sensing and displaying historical event logs and values of components and sensors within the Eclipse 5 system. This can be used to determine system faults or user errors and communicate data for troubleshooting or documentation related to service and updates. EDAT hardware attaches or Plugs into the Eclipse 5 Service Port, and into a computer's USB port.

The EDAT software set allows a provider to set-up a hub and spoke service center. Field service reps can travel to a patient's home, troubleshoot and transmit the data to either in-house tech support personnel or CAIRE Support personnel can diagnose, provide solutions and print documentation for equipment records.

EDAT also makes Eclipse 5 software upgrades easy and accessible.

For more information on EDAT, contact CAIRE Inc. Technical Service at 1-800-482-2473 and reference EDAT PN 5535-SEQ.

POWER SUPPLIES

The Eclipse 5 may operate from either the AC or DC Power Supply or the Power Cartridge. When power is available from an external supply, the Eclipse 5 will draw from the external source rather than depleting the Power Cartridge. Connection to external power is indicated when the External Power Present Indicator located on the Control Panel is illuminated.

AC POWER SUPPLY

The AC Power Supply is a universal input type, capable of accepting **100-240VAC, 50/60 Hz**. It is capable of delivering up to 200W of 28VDC output. The input cord requires a grounded receptacle. Country specific cords or universal power adapter PN 5591-SEQ may be used with the AC Power Supply, as the power supply is equipped with a universal input receptacle. When used in a medical care facility, international safety standards require the use of hospital grade AC power cord with the Eclipse 5.



Figure 5: Eclipse 5 AC Power Supply

The Eclipse 5 AC Power Supply does not contain a fan. When in use, the AC Power Supply should be located in a well-ventilated area.

Located near the output cord, there is a green LED that is illuminated when the AC Power Supply is supplying 28VDC power. If the LED is not illuminated, there is no input power available. In addition, the Power Supply contains protection circuits for output over-current, input over-voltage, and internal over-temperature conditions. If any of these conditions exist, output power will be interrupted and the LED turns off. However, these three conditions are self-resetting, such that output power will resume when protection circuits fall back into acceptable operating ranges.

Note:

Eclipse 5 models with 3 LEDs can use the newer 2-pin power supply (PN: 20852326S (with IEC type A cord), 20852325S (with IEC type C cord), and 20852324S (with IEC type G cord)). In order for the Eclipse 5 models with 2 LEDAs to be used with the older 3-pin power supply (PN 5941-SEQ), the CSA labeling would need be removed from the unit. The applied part would then change from type BF to type B.

DC POWER SUPPLY

The DC Power Supply is intended for use with DC accessory outlets, such as those found in motor vehicles. Input voltage to the DC Power Supply is 11.5-16 VDC. Sized to be compatible with most passenger vehicle electrical systems, it is capable of delivering up to 150W of 26VDC output to the Eclipse 5.



Figure 6: Eclipse 5 DC Power Supply

Located near the output cord, there is a green LED that is illuminated when the DC Power Supply is supplying 26VDC power. If the LED is not illuminated, there is no input power available. The Power Supply contains protection circuits for output over-current, input over-voltage, and internal over-temperature conditions. If any of these conditions exist, output power will be interrupted and the LED will turn off. These three conditions are self-resetting, and output power will resume when protection circuits fall back into acceptable operating ranges.

The Eclipse 5 will run at all flow settings when being operated with the DC power supply in a vehicle including 3.0LPM on continuous flow and all pulse settings 1-9. The Eclipse 5 will charge the power cartridge while being operated with the DC power supply while running at 2.0LPM or below with continuous flow. The power cartridge can charge at all pulse flow rates, however charging functionality may stop depending on the breathing rate of the user. If the Eclipse 5 power cartridge is being charged, the battery symbol will display with a waterfall animation. However, if the power cartridge is not charging then the battery symbol will remain steady and display the current charge capacity.

DO NOT use the DC supply to power the Eclipse 5 once the vehicle's engine is turned off as this may drain the car's battery.

POWER CARTRIDGE (BATTERY)

The Power Cartridge allows operation away from AC or DC power. The Power Cartridge used with the Eclipse 5 contains Lithium ion battery cells, similar to those used in laptop computers and cell phones. The Eclipse 5 Power Cartridge contains a quantity of two 97.5 Watt hour battery packs. Each battery pack contains 7.92 grams of equivalent lithium content.



Figure 7: Eclipse 5 Power Cartridge

The Power Cartridge (Battery) may be charged in two ways: (a) place the Power Cartridge in the Eclipse 5 and connect the Eclipse 5 to AC or DC power, or (b) place the Power Cartridge in the optional Desktop Charger (PN 7112-SEQ).

Operating and servicing the Power Cartridge will ensure longer life and higher performance. It is important to follow the tips and recommendations when storing and operating the Eclipse 5 on the Power Cartridge.

The Eclipse 5 Power Cartridge operation time may be affected by several factors such as bolus size, breathing rates, ambient temperature, age of power cartridge and use over time. The table below describes the typical operating time for a new Power Cartridge.

If the Eclipse 5 is used in Pulse Dose Mode, there will be longer operating time. The patient should consult their physician for a prescription for Pulse Dose Mode.

TYPICAL NEW POWER CARTRIDGE OPERATING

(At nominal temperature of 25°C/77°F)

| Continuous Flow Setting | Battery Duration | Pulse Setting | Battery Duration (12 BPM) |
|-------------------------|------------------|---------------|---------------------------|
| 0.5 LPM | 4.4 hours | - | - |
| 1.0 LPM | 3.7 hours | 16mL 1.0 | 5.4 hours |
| 2.0 LPM | 2.0 hours | 32mL 2.0 | 5.1 hours |
| 3.0 LPM | 1.3 hours | 48mL 3.0 | 4.9 hours |
| | | 64mL 4.0 | 4.0 hours |
| | | 80mL 5.0 | 3.7 hours |
| | | 96mL 6.0 | 3.5 hours |
| | | 128mL 7 | 2.5 hours |
| | | 160mL 8 | 2.0 hours |
| | | 192mL 9 | 1.7 hours |

Battery Consumption Chart

NOTE: Battery times will decrease with higher bolus size, breath rate, ambient temperature, Battery age and use over time.

The Power Cartridge packaged with the Eclipse 5 is not fully charged. Before using the Eclipse 5 Oxygen System for the first time, the Power Cartridge must be fully charged.

Store the power cartridge in a cool, dry location. Do not leave the Eclipse 5 or Power Cartridge in a vehicle or trunk during a hot or cold day.

When checking the Eclipse 5 as baggage on a commercial airline flight for international travel, remove the Power Cartridge and properly package.

When shipping the Eclipse 5 for any reason, remove the Power Cartridge from the Eclipse 5.

If the Power Cartridge gets too warm, charging will not begin until the Power Cartridge sufficiently cools. Consider removing the Power Cartridge to allow for faster cooling.

The Power Cartridge operating time is longer if the Eclipse 5 is operated in Pulse Dose Mode. (Refer to Battery Consumption Chart above.)

The typical time to recharge the Power Cartridge to achieve 80% capacity from a fully discharged Power Cartridge is 1.8 hours to 5.0 hours, dependent upon the flow setting.

The capacity of the Eclipse 5 Power Cartridge is determined by electronics and the Eclipse 5 software.





| | | |
|----------|---|---|
| WARNING: |  | DO NOT tamper with, disassemble, crush or heat the Power Cartridge above 140° F (60° C). The Power Cartridge may present a risk of fire or explosion and will void the warranty. |
| | | |
| CAUTION |  | Store the Power Cartridge in a cool, dry place when not in use. |
| | | |
| CAUTION |  | DO NOT leave the Eclipse 5 or the Power Cartridge in a vehicle or in the trunk during a hot or cold day. |
| | | |
| CAUTION |  | The Eclipse 5 system can only work with a CAIRE Power Cartridge. Use of another Power Cartridge or Battery may damage the unit, present a risk of fire or explosion and will void the warranty. |
| | | |



Figure 8: Power Cartridge Status Gauge (3 LED model pictured. 2 LED model does not have red LED.)

While the Eclipse 5 Power Cartridge allows the concentrator to operate at its full range of capabilities, the primary purpose of the Power Cartridge is to allow a patient to ambulate while they are moving between stationary power sources. The Eclipse 5's Power Cartridge, like all lithium ion batteries, is susceptible to permanent damage from excessive heat. Exposure to excessive heat may significantly shorten the service life of the Power Cartridge.

Each Power Cartridge contains multiple temperature sensors to monitor battery cell temperature. The amount of heat the Power Cartridge can safely endure varies depending on how the Power Cartridge is being used. During discharge, the Eclipse 5 software will alarm when internal battery cell temperature exceeds 60°C, and will shut the system down if internal battery cell temperature exceeds 70°C. While the Power Cartridge is charging, software will interrupt charger operation when the internal battery temperature exceeds 45°C or temperature is less than 0°C. In both of these cases, when internal battery cell temperature falls within these limits, the Eclipse 5 will resume normal operation. Operation near these temperature limits will not damage the Power Cartridge, but are in place to ensure that the service life of the Power Cartridge is preserved.

Heat in the Power Cartridge is generated during discharge, and can also be the result of operating the Eclipse 5 in high ambient temperatures. The amount of internally generated heat varies with the flow setting – higher flows induce greater Power Cartridge heating. While high ambient temperatures are typically the result of operation on a hot day, running the Eclipse 5 with inadequate ventilation can also add additional heat. Always ensure that the Eclipse 5 is operated in a well-ventilated space, the air intake filter is clean, and intake and exhaust vents are unobstructed.

CHARGING ALGORITHM

The charging algorithm is performed by the Power Manager software and involves three basic decisions:

1. When to start charging
2. How fast to charge
3. When to stop charging

Charging begins when Power Cartridge voltage falls below 16.0 volts.

The charging current is limited by the charger capability and the rated capacity of the Power Cartridge. Under certain conditions, the Eclipse 5 may not have enough external power available to charge the batteries at the full rate. In this case, the charging rate will be limited to the available power.

As the Power Cartridge accumulates charge, the charging current required will eventually fall. When the charging current for each Power Cartridge has fallen below 5% of the rated capacity, charging is complete and the Power Cartridge charger is shut off.

The software will only charge when the Power Cartridge temperature is at or below 45°C. The software will always run the cooling fan whenever the charger is enabled. The Power Cartridge charger is disabled and the cooling fan is set to maximum whenever the Power Cartridge temperature exceeds 45°C. The Power Cartridge charger is disabled when temperature is less than 0°C.

All lithium ion batteries self-discharge at very low rates when not in use. Eclipse 5 Power Cartridges are shipped from CAIRE Inc. in a partially charged state (nominally 40%). When stored in a cool, dry location, the Power Cartridge can sit unused for up to 12 months without appreciable self-discharge occurring. Nevertheless, CAIRE recommends a first in, first out rotation of Power Cartridge inventory for maximum Power Cartridge service life.

Training The Patient

INTRODUCTION

Welcome to the Eclipse 5, Personal Ambulatory Oxygen System with autoSAT Technology. Setting up and training your patient to use the Eclipse 5 has never been easier! You can expect your patients and care providers to easily learn how to use the device by following the directions in this section. While setting up and training a patient, be sure to point out the advantages of the Eclipse 5. For example:

- Slim and sleek appearance
- Easy-to-use controls
- Quiet operation
- Lower electric bills
- Self-monitoring alarm system
- More consistent FiO₂ at higher breath rates

After completing each training procedure, ask your patient if he or she has any questions. Proper training of your patients will result in fewer service calls, improved compliance and increased patient satisfaction.

PRE-DELIVERY CHECK LIST

Before delivering the device, check and log the status of the following:

- **Parts Inventory** – Verify that each Eclipse 5 is provided to the patient with the following items:
 - ✓ Users Manual
 - ✓ Quick Start Guide
 - ✓ Eclipse 5 Passport
 - ✓ Universal Cart
 - ✓ Cannula
 - ✓ AC Power Cord
 - ✓ AC Power Supply
 - ✓ DC Power Supply
 - ✓ Power Cartridge (Battery)
 - ✓ Air Inlet Filter and Spare
- **Power Sources** – Insert and check the following for proper operation:
 - ✓ AC Power Supply with Power Cord
 - ✓ DC Power Supply
 - ✓ Power Cartridge (Battery)
- **Electrical System** – Use the Control Panel to check and/or adjust the following:
 - ✓ Pulse Dose Setting
 - ✓ Continuous Flow Setting
 - ✓ Hour meter
 - ✓ Pulse Dose Sensitivity
 - ✓ Bluetooth (on 2 LED models)
 - ✓ 9V Battery Status
 - ✓ Rise Time
 - ✓ Software Revision
 - ✓ Power Cartridge Status Gauge


The Eclipse 5 is shipped from CAIRE Inc. at default flow settings of 2 LPM Continuous Flow, 2.0 Pulse Dose, and 2 for Pulse Mode Sensitivity Adjustment and FAST Rise Time. You may adjust these settings to your patient's prescription when you deliver and set up the device.

INDICATIONS FOR USE


The Eclipse 5 is indicated for the administration of supplemental oxygen. The device is not intended for life support nor does it provide any patient monitoring capabilities.


A physician must prescribe a specific oxygen flow rate setting to meet patients' individual needs.


Recommended oxygen flow rates should be adjusted only under the advice of a physician.


| | |
|---|--|
| WARNING: | Federal law restricts this device to sell by or on the order of a physician. |
|  | |

CONTRAINDICATIONS

| | |
|---|---|
| WARNING: | The Eclipse 5 is not intended for life supporting or life sustaining applications, nor does it provide any patient monitoring capabilities. |
|  | |

| | |
|---|--|
| WARNING: | In certain circumstances, the use of non-prescribed oxygen can be hazardous. This device should only be used when prescribed by a physician. |
|  | |

| | |
|---|---|
| WARNING: | Not for use in the presence of flammable anesthetics. |
|  | |


| | |
|---|---|
| WARNING: | As with any electrically powered device, the user may experience periods of non-operation as a result of electrical power interruption, or the need to have the Eclipse 5 serviced by a qualified technician. The Eclipse 5 is not appropriate for any patient who would experience adverse health consequences as a result of such temporary interruption. |
|  | |

BASIC CONCEPT TRAINING

The following section is intended to assist the provider to train the patient or caregiver to use the Eclipse 5. Topics in this section should be discussed with each patient prior to release for use of the Eclipse 5.



SAFETY GUIDELINES AND OPERATIONAL SAFETY WARNINGS & CAUTIONS

Provider should review all safety guidelines and operational safety Warnings/Cautions with each patient. In addition, provider should carry out a risk assessment prior to installation of the Eclipse 5 to assure proper connection and compatibility with other equipment the patient may be using.

| | |
|---|--|
| WARNING: | <p>No Smoking or Open Flames. For safety concerns, all possible sources of ignition must be kept away from the oxygen system and preferably out of the room in which it is being used. Smoking in the proximity of an operating oxygen concentrator is dangerous and can permanently damage the device and void the warranty. Keep the Eclipse 5 at least five (5) feet (1.5 m) from heat sources, sparking objects or open flames.</p> |
|  | |


LOCATING THE ECLIPSE 5 FOR PROPER USE AND VENTILATION

Ask your patient where they would like to set up the device. Whenever possible, the Eclipse 5 should be in the same room as the patient for convenience and assurance that the patient can adequately hear and respond to Eclipse 5 alerts and alarms. While unpacking and setting up the device, tell your patient about these important cautions and warnings:

| | |
|---|---|
| WARNING: | <ul style="list-style-type: none"> Locate the Eclipse 5 in a well-ventilated space that provides adequate airflow. Ensure that furniture, draperies or clothing will not impede air circulation. Avoid placing the unit over a floor heat register or against a baseboard heating system. Do not use in the presence of flammable anesthetics, solvents, aerosols or flammable cleaning agents. Avoid high pollutant environments. |
|  | |
| CAUTION | <p>Some patients are highly mobile and may use the device under varying circumstances. Make sure your patient or patient caregiver completely understands the basic precautions to safely locate the device.</p> |
|  | |
| NOTE: | <p>After completing this training procedure, ask your patient if s/he has any questions.</p> |

THE USERS MANUAL

Give your patient a copy of the Eclipse 5 User’s Manual and advise them to read prior to operating. Open the manual and briefly review the Table of Contents, including subheadings. Show your patient the icons and symbols and explain what each means.


| | |
|---|---|
| CAUTION | <p>Advise your patient to thoroughly read the Eclipse 5 User’s Manual and keep the manual in a safe place for future reference.</p> |
|  | |

SHOWING PANEL BUTTONS, INDICATORS, ALERTS AND ALARMS

Open the User’s Manual to the section on “UNDERSTANDING THE CONTROLS AND FRONT PANEL” and show your patient where each button is located on the Eclipse 5 Control Panel and how each button and indicator operates. Go over the alerts and alarms and how to handle alert and alarm conditions. Detailed instructions for each button and indicator can be found in the Eclipse 5 User’s Manual.


SHOWING POWER CARTRIDGE POWER LEVEL

The display on the Control Panel shows the amount of Power Cartridge capacity available and waterfalls when charging. Point out the table showing typical new Power Cartridge duration-of-use time in the User's Manual.

| | |
|---|---|
| WARNING: | <p>The display gives an <i>approximate</i> level of remaining battery power. If the patient is dependent on oxygen therapy, the users should always have a backup oxygen supply or access to AC or DC Power Supply in the event of loss of battery power.</p> |
|  | |


SELECTING THE PROPER FLOW MODE AND SETTING

The recommendations of the qualified clinician responsible for the patient's care should always be followed when instructing patients on the use of Continuous or Pulse Dose Mode.

| | |
|---|--|
| WARNING: | <p>Do not attempt to prescribe oxygen level settings. Warn your patient that only a qualified clinician or physician is qualified to perform the necessary tests to prescribe treatment.</p> |
|  | |


SELECTING CONTINUOUS FLOW MODE

When delivered from CAIRE Inc., the Eclipse 5 is set to Continuous Flow Mode. Refer your patient to the User's Manual for instructions on how to select Continuous Flow Mode. Demonstrate the procedure on the device. Set the prescribed flow using the increase or decrease flow rate buttons

| | |
|---|--|
| CAUTION | <ul style="list-style-type: none"> • Continuous Flow Mode is required in order to use a humidifier bottle. • Continuous Flow Mode without a humidifier bottle is required in order use 50 foot tubing. |
|  | |

SELECTING PULSE DOSE MODE

Pulse Dose Mode, delivers a measured bolus of oxygen pulse at the beginning of each inspiration. Refer to the User's Manual for instructions on how to select Pulse Dose Mode. Demonstrate the procedure for your patient. Set the prescribed flow using the increase or decrease buttons. Verify that the patient is able to adequately trigger the oxygen delivery while speaking, sitting quietly, and walking. If the patient is not able to satisfactorily trigger oxygen delivery, the Pulse Sensitivity may need to be adjusted.

| | |
|---|---|
| CAUTION | <ul style="list-style-type: none"> • Do not use a humidifier when in Pulse Dose Mode. • Use only a 7-foot cannula when in Pulse Dose Mode. Do not use a tubing extension. |
|  | |

Review with the patient the breath rate capabilities of Pulse Dose Mode for their prescription.

See Table on page 7

‘POWER CARTRIDGE (BATTERY) CONSERVATION’ FEATURE


While in Pulse Dose Mode, the Eclipse 5 is always monitoring for breath detection. After 15 seconds of no breath detected, the Eclipse 5 “delivers” Continuous Flow at the last Continuous Flow setting. The system and display are still in Pulse Dose Mode and the green Delivery Mode Indicator is blinking fast, indicating you are receiving a Continuous Flow. After 15 seconds, the Eclipse 5 stops delivering Continuous Flow and waits 15 seconds for a breath. If a breath is detected, then the Eclipse 5 will go back to Pulse Dose Mode. If a breath is not detected, the Battery Conservation function will continue; 15 seconds Continuous Flow, 15 seconds Pulse Dose Mode. The Eclipse 5 will stay in this modality until a breath is detected.

This power management feature of the Eclipse 5 greatly conserves the operating life of the battery, extending therapy time and patient mobility.

ADJUSTING THE PULSE DOSE MODE SENSITIVITY SETTING

The oxygen delivery trigger sensitivity may be adjusted to satisfy patient requirements, by selecting setting 1, 2 or 3 (1=most sensitive, 3=least sensitive). The default setting for units coming from CAIRE Inc. is “2”. To adjust the Pulse Sensitivity, perform the following steps:

1. Have the patient sit quietly, with the nasal cannula properly fitted.
2. Put the Eclipse 5 into Pulse Dose Mode at the patient’s prescribed flow setting.
3. Press the “No Smoking” icon until the “PS=”value is displayed.
4. Press the “+” or “-” buttons to raise or lower the sensitivity (1=most sensitive, 3=least sensitive.)
Raising the sensitivity will require additional inspiratory effort to trigger the oxygen pulse. Lowering the sensitivity will require less inspiratory effort to trigger the oxygen pulse.
Too low of a setting may result in false triggering.
5. Verify that the patient is able to adequately trigger the oxygen delivery while speaking, sitting quietly, and walking. Steps 1-6 may be repeated until the patient is able to adequately trigger oxygen delivery.

| | |
|---|---|
| WARNING: | As with all conserving devices, the Eclipse 5 may not be able to detect some respiratory efforts. |
|  | |

| | |
|--------------|--|
| NOTE: | The Eclipse 5 requires a minimum of one minute to stabilize after a change. After a setting change, always wait at least one minute before determining if another adjustment is necessary. |
|--------------|--|


ADJUSTING RISE TIME

The adjustable Rise Time feature on the Eclipse 5 was designed for patient comfort. The Rise Time feature adjusts flow and speed of bolus delivery, and determines how quickly the patient receives their bolus volume while in Pulse Dose Mode. The Eclipse 5 offers delivery settings of FAST, MEDIUM, and SLOW. The factory default setting is FAST. A MEDIUM or SLOW rise time may be appropriate for certain patients, and should be determined and set by a trained clinician. Adjusting the Rise Time will not affect the chosen volume of oxygen delivered to the patient (16-192 mL).


CONNECTING THE AC POWER SUPPLY


The Eclipse 5 operates from external power when connected to a power outlet.

To connect the Eclipse 5 to the AC Power Supply, follow these steps:

1. Insert the AC supply plug tip into the Eclipse 5.
2. Insert the power cord into the AC Power Supply.
3. Plug the power cord into a grounded outlet.
4. The power supply LED displays green to indicate that the AC Power Supply is drawing power. The External Power Present Indicator on the Control Panel illuminates. 

| | |
|--------------|---|
| NOTE: | If the Power Supply Status LED is not illuminated after inserting the plug into a grounded outlet, check to make sure the Power Supply and power cords are securely plugged into the Eclipse 5. |
|--------------|---|

| | |
|---|--|
| WARNING: | <ul style="list-style-type: none"> • Ensure adequate clearance around the AC Power Supply. • The AC Power Supply is universal input, but the AC power cord is appropriate to specific country's electrical service. Ensure that power cord is appropriate to country's electrical service. |
|  | |

| | |
|---|--|
| CAUTION | <ul style="list-style-type: none"> • DO NOT connect the Eclipse 5 to an extension cord or electrical outlet controlled by a switch. |
|  | |


| | |
|--------------|---|
| NOTE: | When removing the AC Power Supply from the Eclipse 5, remove the plug from the AC outlet before removing the AC Power Supply plug from the Eclipse 5. |
|--------------|---|

International safety standards require the use of hospital grade AC power cords (3893-SEQ) when using the Eclipse 5 in a medical care facility. Contact CAIRE Inc. to obtain a hospital grade AC power cord for the Eclipse 5 if necessary.

CONNECTING THE DC POWER SUPPLY



To install the DC Power Supply, follow these steps:

A DC Power Supply allows the system to operate from DC outlets, such as those found in motor vehicles.


| | |
|---|--|
| CAUTION | <p>The DC Power Supply is designed for 12VDC minimum vehicle electrical systems. Do not attempt to operate with 6V, 24V, or other vehicle electrical system.</p> |
|  | |

1. Consult your patient's vehicle owner's manual for DC Accessory outlet requirements.
2. Secure your Eclipse 5 and DC Power supply in your vehicle. Ensure that alerts and alarms are observable.
3. Start the vehicle's engine.
4. Insert supply plug into DC accessory outlet.
5. Attach the Power Supply plug to the Eclipse 5.
6. Advise the patient to use Pulse Dose Mode if prescribed by their clinician.
7. When the device is properly connected and receiving power from the DC power source, a green indicator light on the DC Power Supply will illuminate.

Ask your patient whether he or she will be using the device to travel by vehicle. If so, show your patient how to safely use the Eclipse 5 while driving. Refer to the previous section on Connecting the DC Power Supply for proper setup of the Eclipse 5 system in a vehicle.


| | |
|---|---|
| WARNING: | <ul style="list-style-type: none"> • Ensure adequate clearance around the DC Power Supply and the Eclipse 5. • Ensure the DC Power Supply and Eclipse 5 are secured in the vehicle so that it does not become a projectile in the event of a sudden stop. • DO NOT operate the Eclipse 5 on DC power while the vehicle engine is off. In such a scenario, the Eclipse 5 could quickly drain the vehicle's battery. |
|  | |
| CAUTION | <p>When operating an Eclipse 5 with the DC power supply, the power cartridge will only recharge if there is sufficient excess voltage from what the concentrator requires to operate.</p> |
|  | |

When the Eclipse 5 is running from an external (AC or DC) power supply, the External Power Present Indicator will illuminate.

 The Eclipse 5 will always operate from external power when external power within the specified range is available.

ACTIVE LIFESTYLE TRAINING


Small, lightweight, and easily moved about, the Eclipse 5 is ideally suited to an active lifestyle. The AC and DC supplies enable recharge of the Power Cartridge during longer excursions and even extended overnight travel. To train your patient on mobility and ambulation, follow the procedures below.

| | |
|---|---|
| CAUTION | Always check to see that the Air Inlet and the Exhaust Vent are not blocked and the Air Inlet Filter is dry and clean before using your Eclipse 5. |
|  | |
| NOTE: | <ul style="list-style-type: none"> • Do not drop the Eclipse 5 or Eclipse 5 power supplies. If dropped or damaged, verify unit performance. • The Eclipse 5 will not detect a cannula that has been disconnected from the Oxygen Outlet Port. |

ATTACH THE UNIVERSAL CART


Your patient will enjoy the mobility offered by the Eclipse 5 Universal Cart in and outside the home. Show your patient how to perform the following important activities:

- Mounting the Eclipse 5 to the Universal Cart
- Extending and collapsing the telescoping handle

| | |
|---|---|
| CAUTION | Do not lift the Eclipse 5 by the cart handle. |
|  | |

USING AROUND THE HOUSE

Your patient may use 50' tubing when operating the Eclipse 5 in the house. In order to use extended tubing, the device must be in Continuous Flow Mode. When a humidifier is used, the tubing between it and the patient must not exceed 7'.

| | |
|---|---|
| CAUTION | When using a humidifier adapter of any kind, the Eclipse 5 unit must remain stationary, meaning that the unit must NOT be moved or transported in any manner. |
|  | |


TRAVELING BY VEHICLE


Ask your patient whether he or she will be using the device to travel by vehicle. If so, show your patient how to safely use the Eclipse 5 while driving. Refer to the previous section on Connecting the DC Power Supply for proper setup of the Eclipse 5 system in a vehicle.

| | |
|-------|--|
| NOTE: | Whenever possible, go to your patient's vehicle to demonstrate this procedure. |
|-------|--|



Figure 9: Eclipse 5 DC Power

| | |
|---|--|
| CAUTION | Be sure to accurately determine the amount of current the vehicle accessory outlet is rated to supply. |
|  | |

| | |
|---|--|
| WARNING: | <ul style="list-style-type: none">• Avoid placing the Eclipse 5 in direct sunlight.• Do not store the Eclipse 5 in a vehicle where the device may be subject to extreme temperatures. Extreme heat or cold may impair operation and damage the device and degrade the Power Cartridge.• When using the Eclipse 5 in a vehicle, check the cannula to make sure it is not pinched or occluded. |
|  | |

TRAVELING BY AIR

TRAVEL APPROVED

The Eclipse 5 is an FAA approved portable concentrator.

A new US Department of Transportation regulation regarding portable oxygen concentrators took effect on May 13, 2009. Under this regulation, every FAA approved portable concentrator is now authorized for use during any commercial flight that departs or arrives in the USA, regardless of whether the airline itself has approved the device or not.

When traveling by air, instruct your patient to remove the Power Cartridge from the Eclipse 5 before checking the unit as checked baggage or cargo. Transport of the Eclipse 5 as cargo or checked baggage with the Power Cartridge installed is prohibited by international air cargo regulations.

The Power Cartridge may be installed if the patient is using the Eclipse 5 as a carry-on item.

If the airline allows use of the Eclipse 5 Oxygen System, only operate the Eclipse 5 from the Power Cartridge. **DO NOT** use DC or AC Power Adapters on an aircraft. The patient must ensure that they have an adequate number of spare Power Cartridges to last for the duration of their trip.

During taxi, take-off and landing the Eclipse 5 must be turned off and stowed under the seat or in another approved stowage location as to not block the aisle way or the entry way into the row if the Eclipse 5 will not be used.

During taxi, take-off and landing the user must be in a seat location that does not restrict any other passenger's access to, or use of any required emergency or regular exit, or the aisle(s) in the passenger compartment of the aircraft if the Eclipse 5 is used.

Users are not permitted to be seated in an exit row if using the Eclipse 5.

If the Eclipse 5 is used when decompression of the cabin occurs and the oxygen cabin oxygen system deploys, then the user is to use discontinue use of the Eclipse 5 and use the aircraft supplemental oxygen. The Eclipse 5 unit is to be turned off after securing the aircraft supplemental oxygen.

Prior to travel the user needs to inspect the Eclipse 5 to ensure in good operational condition.

Visit our website, www.sequal.com to the Travel Approved section, for helpful travel tips, forms used to assist with traveling and estimated number of Power Cartridges (batteries) needed for flights.

Each airline has their own requirements and CAIRE recommends checking those requirements prior to making a trip.

TRAVELING BY CRUISE SHIP

When traveling by watercraft, instruct your patient to inform the cruise line that the Eclipse 5 will be used onboard. Each cruise line has a Special Needs coordinator that can answer any questions regarding travel and the cruise line's individual requirements. Have your patient contact the cruise ship Special Needs Coordinator directly.

TRAVELING BY TRAIN

When traveling by train, instruct your patient to inform the rail line in advance that the Eclipse 5 will be used onboard. Operate the Eclipse 5 only from the Power Cartridge. The patient must ensure that they have an adequate number of spare Power Cartridges to last for the duration of their trip.

ECLIPSE 5 MAINTENANCE

WEEKLY MAINTENANCE—PATIENT

Training your patient to maintain the Eclipse 5 properly will lead to longer service intervals and lower maintenance costs. Train your patient to perform the following procedures:

CLEAN THE AIR INLET FILTER


The Air Inlet Filter, located at the rear of the unit, must be cleaned at least once a week.

To clean the filter:

1. Remove the filter from the back of the cabinet.
2. Wash the filter in warm water using a mild detergent solution.
3. Rinse the filter thoroughly and squeeze out the excess water.
4. Allow the filter to air dry thoroughly.
5. Re-insert the filter in the cabinet.
6. Maintenance may be easier for the patient when a second filter is provided.



Figure 10: Cleaning the Air Inlet Filter

| | |
|--|---|
| <p>CAUTION</p>  | <ul style="list-style-type: none"> • The filter should be completely dry before using it again. Excess moisture may impair proper operation or damage the unit. • Replace the Air Inlet Filter annually. If the Eclipse 5 is operated in a dusty environment, the filter may need to be cleaned or replaced more often. Do not operate the Eclipse 5 for more than 30 minutes without a filter installed. |
|--|---|

CLEAN AND CARE FOR THE TUBING AND CANNULA

Provide your patient instructions on cleaning, disinfection and/or replacement information for the tubing and cannula.

CLEAN THE CABINET AND CONTROL PANEL AND POWER SUPPLIES

To clean the cabinet, Control Panel or power supply, do the following:

1. Turn OFF the Eclipse 5 and disconnect from AC or DC power before any cleaning or disinfection activity.
2. Use mild detergent and water solution.
3. Use a damp (not soaking wet) cloth or sponge.
4. Spray or wet the cloth or sponge with the mild detergent solution. DO NOT spray the cabinet, Control Panel or power supplies.
5. Wipe down the cabinet, Control Panel or power supplies.
6. To disinfect the Eclipse 5, use Lysol[®] Brand II disinfectant (or equivalent). Spray or wet a cloth or sponge with the disinfectant. DO NOT spray the cabinet, Control Panel or power supplies. Proceed as directed by the manufacturer.

Note: Only use disinfectants or cleaning agents approved for use with this equipment by CAIRE such as Lysol[®], HydroPure[®], Hydroklean[®] or others as specified by CAIRE.


MONTHLY MAINTENANCE—PATIENT

CARE FOR THE POWER CARTRIDGE

The Power Cartridge (battery) in the Eclipse 5 requires special care to assure a longer life and the highest level of performance. The CAIRE Power Cartridge is the only approved Power Cartridge recommended for use with the Eclipse 5. The following are generic guidelines for the Power Cartridge:

- Avoid high temperatures
- Avoid cold temperatures
- Do not drop Power Cartridge
- No not poke objects into contacts

Power Cartridge Cleaning: Use a damp (not soaking wet) cloth or sponge. First spray the cloth or sponge with a mild detergent and then clean the Power Cartridge case and the latch.

| | |
|---|--|
| WARNING: | Exposing the Power Cartridge to water or other liquids may cause personal injury or harm. |
|  | DO NOT tamper with or try to repair the Power Cartridge. There are no serviceable parts inside. |

Power Cartridge Storage: The Power Cartridge should be stored in a cool and dry location.

CALIBRATING THE POWER CARTRIDGE

In order to maintain the Power Cartridge, your patient should fully discharge the Power Cartridge once a month. In order to accurately maintain the Eclipse 5 Power Cartridge, periodic full discharge of Power Cartridge to zero is recommended. This serves to calibrate the Power Cartridge Status Indicator. To do this, the patient will need an AC Power Supply to recharge the Power Cartridge and should be able to run the Eclipse 5 from AC power for at least 5 hours.

| | |
|--------------|--|
| NOTE: | The patient can still use the Eclipse 5 while zeroing the Power Cartridge. |
|--------------|--|

The patient should follow these steps:

1. Install the Power Cartridge in the Eclipse 5
2. Remove external power and operate the Eclipse 5 from the Power Cartridge
3. Allow the Eclipse 5 to completely discharge the Power Cartridge. This is best performed at a setting of 2.0 LPM Continuous Flow. Ten to fifteen minutes before the end of the discharge cycle, the “Low Power Cart- ridge” alert will sound, followed by the “Power Cartridge Shutdown” alarm. If using the Eclipse 5 while discharging the Power Cartridge, **DO NOT** deviate from the patient’s prescription.
4. Press the ON/OFF button to silence the alarm.
5. Allow the cartridge to cool for a minimum of 1 hour prior to recharging.
6. Reattach external power. Verify that the External Power Present Indicator illuminates. Leave the Power Cartridge installed. Note that the Power Cartridge Status Gauge may not indicate charging immediately. When the Power Cartridge reaches proper temperature, charging will begin automatically.
6. Allow Power Cartridge to fully charge, as indicated by the Power Cartridge Status Gauge.

| | |
|--------------|---|
| NOTE: | <ul style="list-style-type: none"> • If the Power Cartridge temperature rises above 45°C (113°F), the Power Cartridge will not charge. • If the Power Cartridge temperature rises above 70°C (158°F), the Power Cartridge will not discharge. |
|--------------|---|

ECLIPSE 5 MONTHLY RUN-TIME PROCEDURE

1. Power on Eclipse 5 using AC Power, DC Power, or Power Cartridge
2. Allow unit to run for a minimum of 2 hours

PATIENT TRAINING CHECKLIST


Use the following checklist as a guide to assist in setup and training a patient on the use of the Eclipse 5™ with autoSAT® Technology and its accessories.

| Patient Name: | |
|--|---------------------------------|
| Eclipse 5 Serial # | DC Power Supply Serial # |
| AC Power Supply Serial # | Power Cartridge Serial # |
| Training Topic | Initials |
| Pre-Delivery Check List | |
| Indications for Use | |
| Contraindications | |
| Basic Concept Training | |
| Advise to read the Users Manual | |
| Go over all accessories included with the Eclipse 5: AC, DC, Power Cord, Cart, Battery | |
| Safety Guidelines and Operational Safety Warnings/Cautions | |
| Locating the Eclipse 5 | |
| Panel Buttons and Indicators | |
| Alerts and Alarms | |
| Power Cartridge Power Level | |
| Selecting Flow Mode and Setting | |
| • Selecting Continuous Flow Mode | |
| • Selecting Pulse Dose Mode with autoSAT Technology | |
| • Adjusting the Pulse Dose Mode Sensitivity Setting | |
| • Selecting Rise Time | |
| • Battery Conservation feature | |
| Connecting the AC Power Supply | |
| Connecting the DC Power Supply | |
| Active Lifestyle Training | |
| Attach the Cart | |
| Changing Power Cartridge (Battery) | |
| Use Around the House | |
| Traveling by Vehicle | |
| Traveling by Air | |
| Traveling by Boat | |
| Traveling by Train | |
| Eclipse 5 Maintenance | |
| Weekly: Clean the Air Inlet Filter | |
| Weekly: Clean and Care for the Cannula | |
| Weekly: Clean the Cabinet and Control Panel | |
| Monthly: Care for the Power Cartridge | |
| Annually: Schedule PM at least once a year | |
| Trained By: | Date: |

Annual Maintenance—Provider

INTRODUCTION

Properly maintaining the Eclipse 5 will ensure longer life and higher performance. Minimum annual maintenance is required.

| | |
|---|---|
| CAUTION | The Eclipse 5 contains electrostatic sensitive components. Do not open or handle except at a static free workstation. Do not remove cover without ESD protection. |
|  | |

ANNUAL MAINTENANCE CHECK LIST

Perform the following maintenance procedures at least once a year or more often, as needed. The frequency of the periodic maintenance should be based on the environment in which the Eclipse 5 is used.

- Replace air inlet filter
- Check Power Cartridge
- Inspect AC and DC Power Supply plugs and cords for damage. Replace as needed
- Verify that the AC and DC Power Supplies operate with the Eclipse 5
- Readjust the Pulse Dose Sensitivity setting between patients as needed
- Readjust the Rise Time setting between patients, as needed
- Replace 9V battery
- Check Universal Cart for functioning wheels and telescoping handle. Replace as needed
- Read and record hour meter
- Check flow rate, purity, Pulse Dose Mode and alarm functions
- Replace compressor intake filter
- Perform electrical safety test (Required only if used in a hospital or institutional setting; not required for home use)
- Replace HEPA filter
- Bluetooth Setting

CHECKING AND REPLACING THE POWER CARTRIDGE

Typically, the Power Cartridge will require no routine maintenance beyond cleaning by the patient and calibration. CAIRE recommends that the Power Cartridge be replaced if there is physical damage to the cartridge enclosure or connector, or if the battery's recharge capacity, after calibration, is 20% less than published values at its given flow rate.

ECLIPSE 5 MONTHLY RUN-TIME PROCEDURE

1. Power on Eclipse 5 using AC Power, DC Power, or Power Cartridge
2. Allow unit to run for a minimum of 2 hours

| | |
|--------------|--|
| NOTE: | This procedure is performed to ensure and prolong the life of your Eclipse 5. This is also an ample opportunity to calibrate the power cartridge of the Eclipse 5. |
|--------------|--|

ANNUAL MAINTENANCE PROCEDURES

The following section lists procedures that are necessary to maintain the Eclipse 5. Service should only be performed by a qualified technician. To perform periodic maintenance, the only tools that should be necessary are:

- #1 Phillips Screwdriver
- Wire-cutting pliers
- Small cable ties
- ESD Mat or approved ESD system

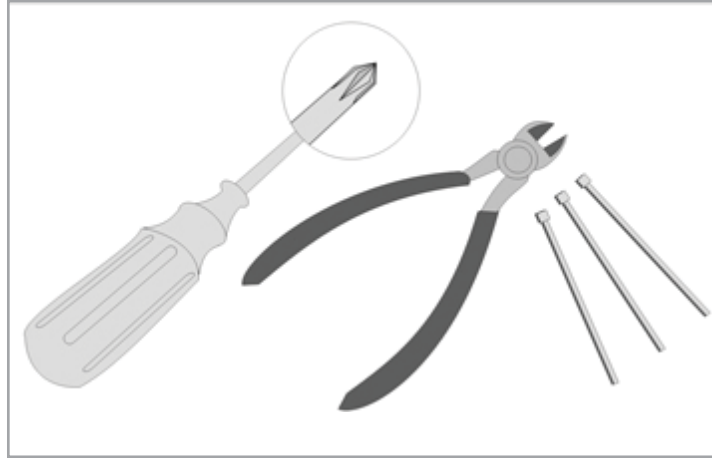



Figure 11: Maintenance Tools.

REMOVING THE UNIT COVER

1. Disconnect power supplies and remove Power Cartridge before removing the unit cover.
2. Place the unit horizontally on the front cover.
3. Using a Phillips #1 screwdriver, remove a total of 10 screws (M3x12 Pan Head SEM Screw, P/N 6974-312-SEQ) from the back of the unit.

| | |
|---|--|
| WARNING: | <ul style="list-style-type: none">• Keep hands out of moving parts• Disconnect power supplies and remove Power Cartridge before removing the unit cover.• ESD Safety procedure must be in place. |
|  | |


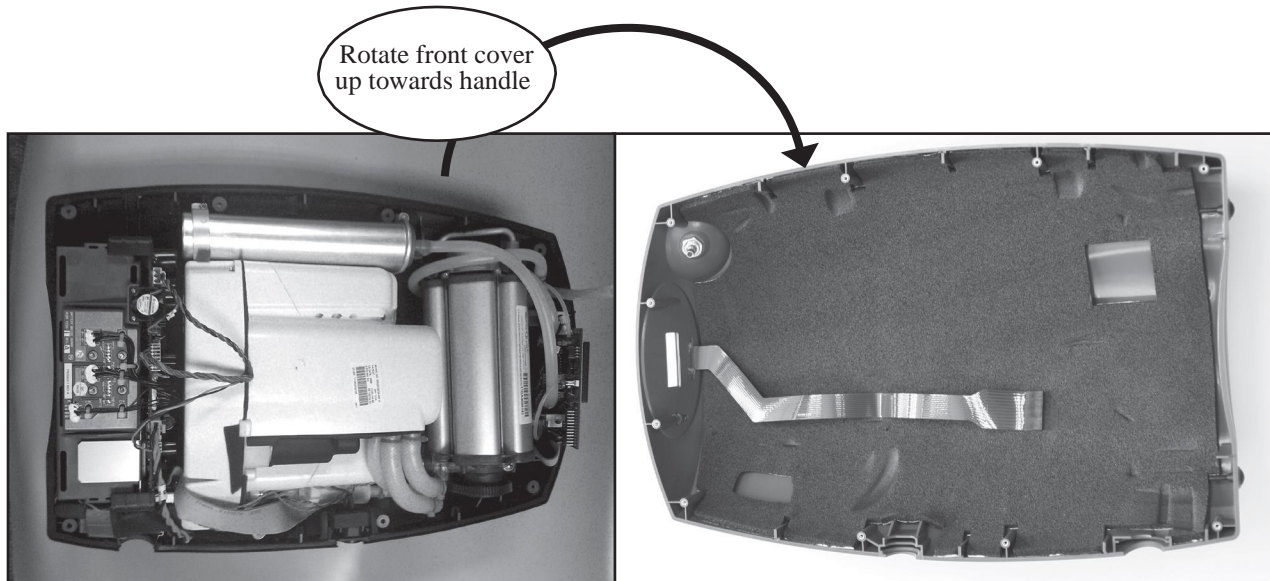
| | |
|---|---|
| CAUTION | The Eclipse 5 contains electrostatic sensitive components. Do not open or handle except at a static free workstation. Do not remove cover without ESD protection. |
|  | |



Figure 12: Removing screws to open the Front Cover


4. Turn over and place the unit horizontally on the back cover.
5. Remove the front cover -- pop the bottom end off first and rotate it towards the handle. Be careful not to tear the Control Panel ribbon cable that is attached to the front cover.

Figure 13: Opening the Front Cover.



6. Disconnect the cable from the Control Panel as follows:

- a. Grasp the circuit board firmly between your fore fingers and thumb.
- b. Grasp the head of the Membrane Panel Overlay cable in your other hand.
- c. Firmly pull the cable away from the board. Pull the cable straight out. Do not rock the connector back and forth. This may damage the pins of the header.

| | |
|---|--|
| CAUTION | Do not disconnect the Membrane Panel Overlay cable by pulling on the ribbon cable. |
|  | |

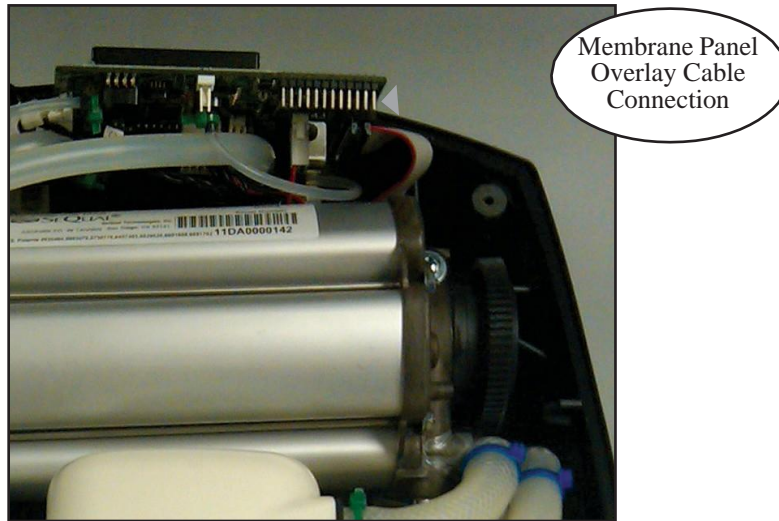



Figure 14: Removing the Membrane Panel Overlay Ribbon Cable.

7. Disconnect the silicone tube from the oxygen outlet tube at the top of the cover. First cut the cable tie, then pull the silicone tube off the oxygen outlet tube.

| | |
|-------|--|
| NOTE: | Always cut the heads of cable ties to avoid damaging the tubing. |
|-------|--|

| | |
|---|--|
| CAUTION | Avoid possible eye injury by wearing protective eyewear or shielding the eyes from possible flying debris. |
|  | |

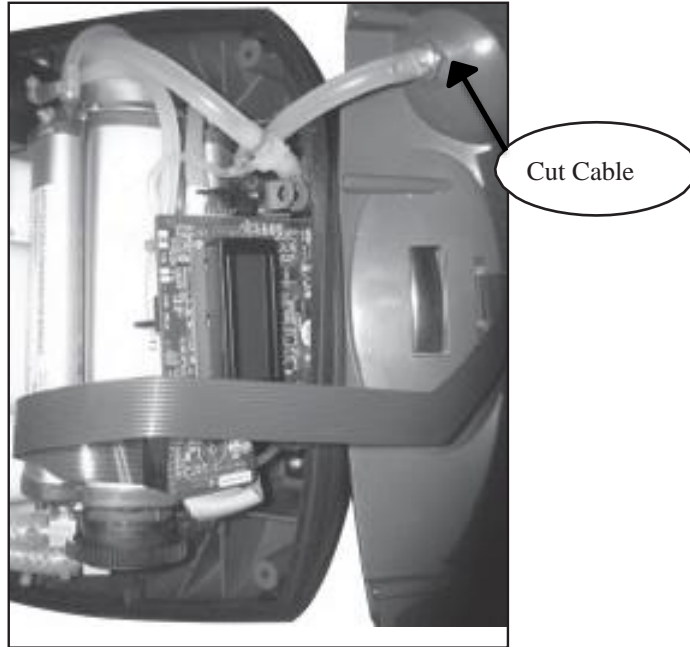


Figure 15: Disconnecting the Oxygen Outlet Tube

8. Lay the front panel away from Eclipse 5. Inspect PEM Nut anchors in the front cover assembly. Perform necessary maintenance.

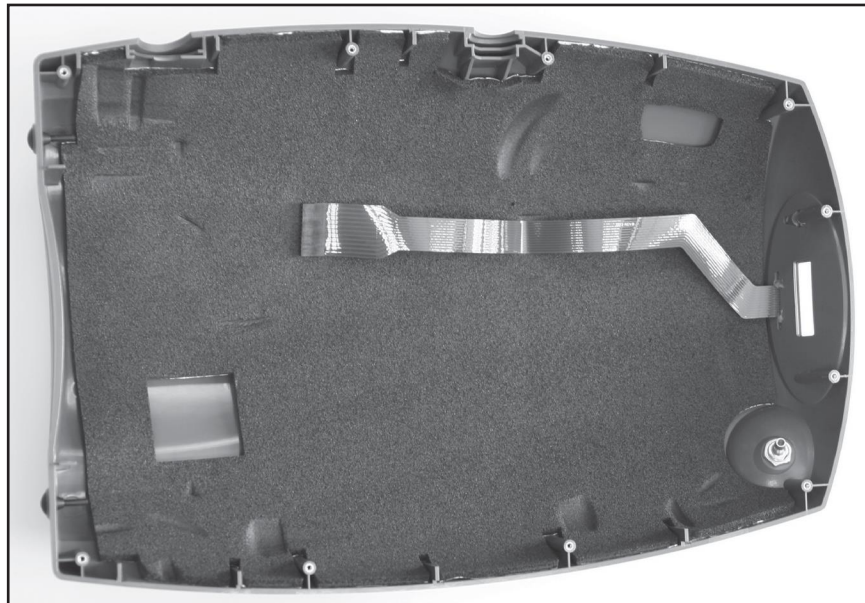



Figure 16: Front Cover Removal

Once the cover has been removed, the procedures listed in this section may be performed.

REMOVE AND REPLACE 9 VOLT BATTERY

Replace the 9-volt battery when the unit beeps three times at the end of power-on self-test, when voltage is less than 7.0 Volts, or during annual PM. To replace the 9-volt battery, follow these steps:

| | |
|---|---|
| WARNING: | Disconnect power supplies and remove Power Cartridge before removing the unit cover. Do not touch exposed circuits during maintenance without ESD protection. |
|  | |

1. Remove the Eclipse 5 front cover assembly.
2. Lift the battery out of the compartment located at the bottom right corner of the unit.

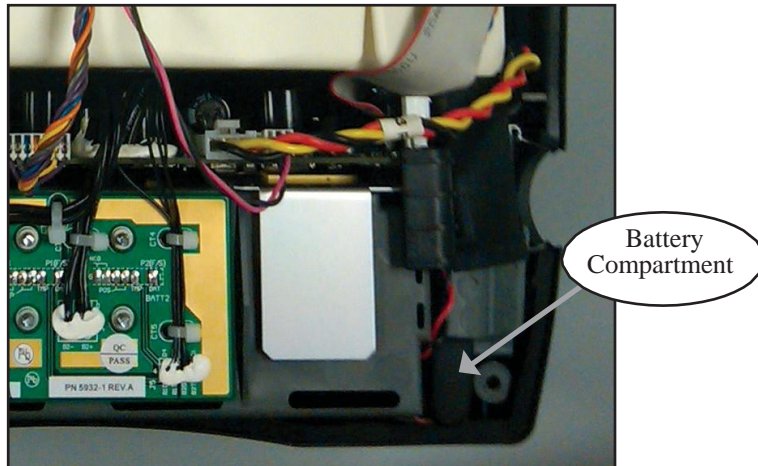


Figure 17: Removing the 9-volt Battery

3. Disconnect the 9-volt battery harness.
4. Remove and replace the 9-volt battery.




Figure 18: Disconnecting the 9-volt Battery.

5. Reconnect the battery harness. Ensure that the terminals are aligned correctly.
6. Place the battery back into the compartment.
7. Install battery foam pad if necessary.

REMOVE AND REPLACE HEPA FILTER

Replace the HEPA filter annually, or more often as needed. To replace the HEPA filter, follow these steps.

| | |
|---|---|
| WARNING: | DO NOT use any petroleum based or other lubricants. A spontaneous and violent ignition may occur if oil, grease or other petroleum substances come into contact with oxygen under pressure. Keep these substances away from the oxygen system, tubing and connections and any other oxygen source. |
|  | |
| NOTE: | Always cut the heads of cable ties to avoid damaging the tubing. |

Internal Filters

HEPA Filter replacement:

1. Cut cable tie and Disconnect the tubing at the top of the filter carriage.



Figure 19: Tubing on Filter Carriage.

2. Unscrew the wing nut that holds the HEPA filter.

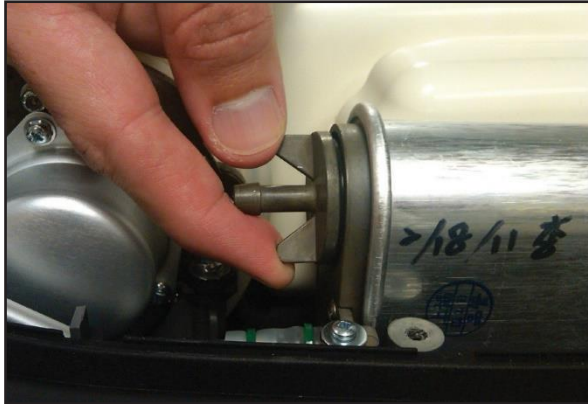


Figure 20: Wing Nut.

3. Unscrew the Clear HEPA filter and discard filter & small o-ring.

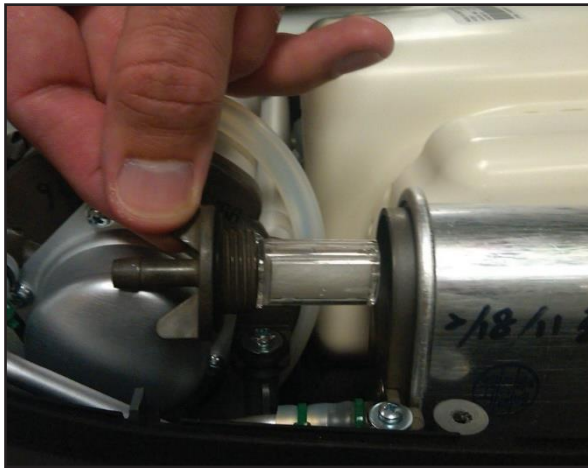


Figure 21: Unscrewing the HEPA Filter.

4. Install the new small o-ring and HEPA filter.



Figure 22: Installing the new HEPA Filter.

5. Locate the large o-ring on the product tank, replace it with the new large o-Ring included in the PM kit (5022-SEQ). Screw the new HEPA filter into the carriage holder (wing nut topped housing). Insert and screw the new HEPA filter (wing nut topped housing) into the carriage holder (product tank) and finger snug in place (do not over-tighten). Re-attach tubing and secure with a cable tie.

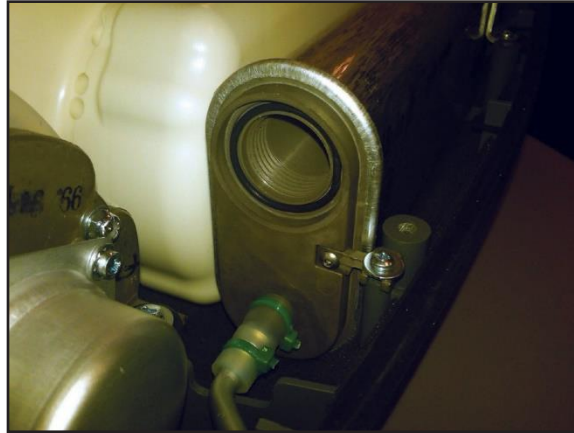



Figure 23: O-Ring.

REMOVE AND REPLACE THE COMPRESSOR INTAKE FILTER

Replace the compressor intake filter annually, or more often as needed. The compressor intake filter may become clogged depending upon the amount of contaminants in the air (smoke, dust, dirt, pollen, etc.) and may need to be changed more frequently. The most common cause of low concentration and eventual system failure is a dirty or clogged compressor inlet filter. Environmental conditions usually determine the effective life of a filter.

| | |
|---|--|
| CAUTION | Operating the Eclipse 5 with a clogged compressor intake filter may reduce performance and lead to system damage or premature failure. |
|  | |

| | |
|-------|--|
| NOTE: | Always cut the heads of cable ties to avoid damaging the tubing. |
|-------|--|

To replace the compressor intake filter, follow these steps:

1. Cut the cable tie on the silicone tubes attached to the compressor intake filter.

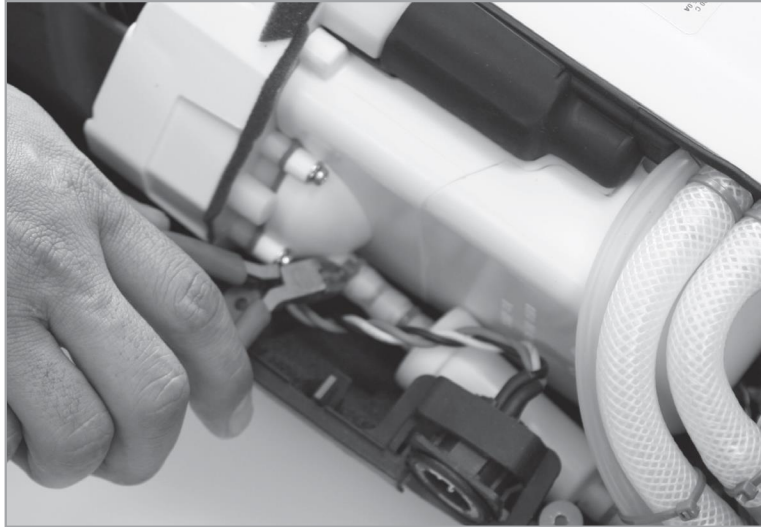


Figure 24: Removing the Compressor Intake Filter.

2. Remove the silicone tubes attached to each end of the filter body.
3. Install a new filter by pushing each tube completely over the barb on the filter body. Verify flow direction is correct.
4. Reconnect silicone tubes to the filter. Ensure that the feed tubes are not blocked, crimped or kinked upon completion of the installation or the unit will alarm for low oxygen purity after the warm-up cycle is complete.



Figure 25: Installing the Compressor Intake Filter.

5. Re-install two cable ties on silicone tubes.

After replacing the Compressor Intake Filter, check the following:

- Verify proper seating of the filter in the Eclipse 5. The arrow on the filter body should point toward the 9-volt battery.
- Ensure that the inlet tube is inserted securely into its hole in the compressor box and is not pinched.

After filter is replaced and unit cover reinstalled, proper functionality should be checked by following the Test Procedures described in this manual.

REINSTALLING OR REPLACING THE UNIT COVER

CAIRE Inc. recommends providers have EDAT (PN 5535-SEQ), or a spare Control Panel (PN SP20618461) that can be attached to the unit, and the unit run for a minimum of 20 minutes prior to re-installing the cover to check for a smooth and quiet calibration to be replaced by operation.

To re-install the cover, follow the steps using the reverse order. Ensure that the Membrane Panel Overlay cable plug is correctly lined up with circuit board connection and that there are no twists in the ribbon cable.

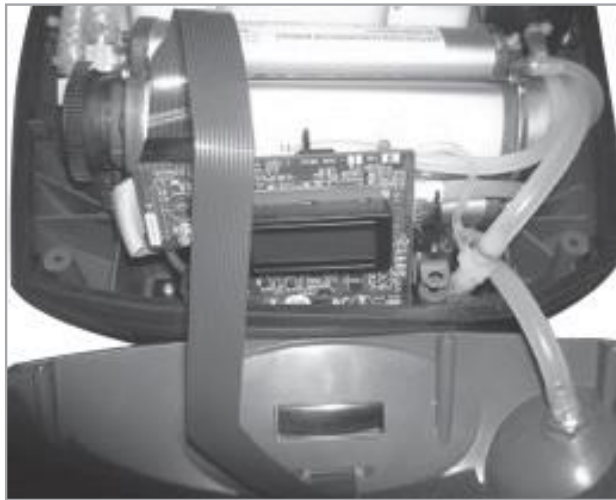


Figure 26: Membrane Panel Ribbon Cable Installation.

Align Front Cover over Control Board and then gently position front cover. Verify that the black rubber gasket (channel seal) and strain relief are aligned and fit properly. Do not over tighten cover screws (5 in. lbs. at maximum).

| | |
|-------|---|
| NOTE: | After the cover has been reinstalled, but before installing screws on the cover, re-connect power and start unit. Let the unit run for 20-30 minutes. |
| NOTE: | Whenever the cover of the Eclipse 5 is removed, proper functionality should be checked by following the Test Procedure described next. |

TEST PROCEDURES

PURITY AND FLOW RATE TEST PROCEDURE - PREFERRED METHOD

It is recommended that the Eclipse 5 be tested for oxygen concentration and flow performance. The CAIRE recommended test setup is shown on the following diagram. Oxygen monitors may or may not have an internal pump to draw samples of oxygen to be measured. Placement of the oxygen monitor in the test setup depends whether they have an internal pump. Only one oxygen monitor is needed. An oxygen monitor such as Salter Labs' PRO₂ Check Elite[®] or equivalent may be used.

- Connect the circuit per the diagram shown below.
- Turn the concentrator on and set the target flow on the Eclipse 5 to 3 LPM continuous flow.
- Allow the Eclipse 5 to stabilize (can take up to 10 minutes).
- Verify the O₂ concentration and O₂ flow rate are within specification (shown in Table 1).

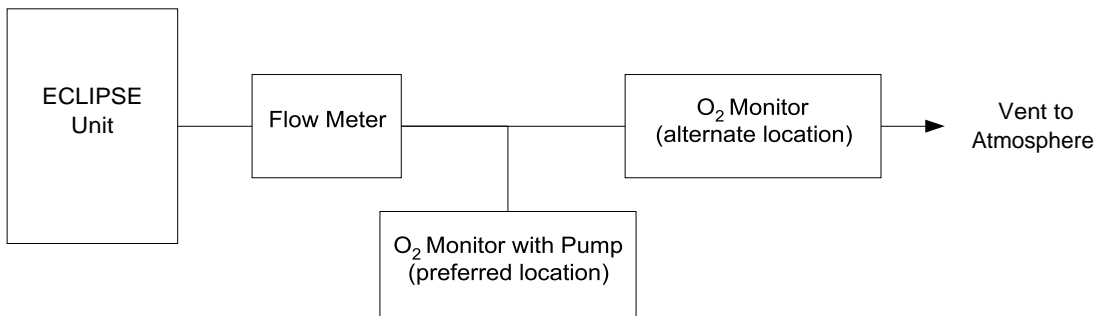


Figure 27: CAIRE Recommended Test Setup to verify performance of Oxygen Concentrator

PURITY AND FLOW RATE TEST PROCEDURE-ALTERNATE METHOD

Attach a calibrated oxygen monitor to the oxygen outlet port in accordance with oxygen monitor manufacturer's recommendations.

| | |
|-------|---|
| NOTE: | Some sensing equipment may restrict the actual flow rate and provide inaccurate concentration readings. If testing is performed with the oxygen monitor in the alternate location pictured above, ensure that the oxygen monitor does not significantly restrict oxygen flow. |
|-------|---|

ASSEMBLY AND ALARM VERIFICATION TESTS

To ensure proper assembly and functionality of the Eclipse 5 after it has been reassembled, the following steps should be followed.

1. Install the Power Cartridge into the Power Cartridge compartment of the Eclipse 5. Plug the AC Power Supply into the wall outlet and connect it to the External Power Connector of the Eclipse 5.
2. Press the ON button and set the Eclipse 5 to 2 LPM. At initial start-up Eclipse 5 units light the Green, Yellow and Red* LED's accompanied by a beep. As concentration increases to ~70%, the Red* LED turns off and the Yellow and Green remain on. When the concentration reaches normal operating range (above 85%), the Yellow LED will turn off. The Green LED will stay lit indicating normal operation. Table 3 shows the normal start-up operating conditions for Eclipse 5 Oxygen Systems. If LED is not green within 7 minutes there may be a problem with the Eclipse 5.

*Later models do not have red LED.

3 LED model

| Green Indicator | Yellow Indicator | Red Indicator | Audible Alarm | Alarm code | Operating Condition |
|-----------------|------------------|---------------|---------------|------------|----------------------------|
| Off | Off | Blinking | Beeps | 004 | Purity < 70% |
| Off | Blinking | Off | Off | 008 | Purity between 70% and 85% |
| On | Off | Off | Off | 000 | Normal Operating Condition |

2 LED model

| Green Indicator | Yellow Indicator | Audible Alarm | Alarm code | Operating Condition |
|-----------------|------------------|--------------------------------|------------|------------------------------|
| Off | On | Beep, repeats every 20 seconds | 008 | Purity < 85% (After warp-up) |
| On | Off | Off | 000 | Normal Operating Condition |

3. Verify that the Power Cartridge is charging as indicated by the Power Cartridge Status Gauge is moving in waterfall fashion (scrolling from bottom to top). If the Power Cartridge Status Gauge is not moving, verify that the Power Cartridge is properly engaged.
4. Check the Control Panel by pressing each of the Increase/Decrease, Pulse Dose Mode and No Smoking buttons and observe that the Eclipse 5 buttons function normally.
5. Press the Delivery Mode button and set the Eclipse 5 to the patient's normal Pulse Dose setting. Confirm that without breathing from the unit, after 15 seconds of no breath detected, the system changes automatically to Continuous Flow Mode. The green Delivery Mode light is blinking fast, indicating the system is delivering a Continuous Flow. After another 15 seconds, the system stops delivering Continuous Flow and waits 15 seconds trying to detect a breath. The cycle continues until a breath is detected.
6. After 5 minutes of operation, block the Cannula Fitting Outlet with your finger for 2 minutes and confirm that the visual and audible alarm occurs. Unblock the Cannula Outlet Port and let it stabilize until the alarm stops.
7. Disconnect the AC Power Supply and allow the Eclipse 5 to run for about one minute. Set the Eclipse 5 to the patient's normal Continuous Mode setting. Confirm that the Power Cartridge Status Gauge is illuminated and External Power Present Indicator is off.
8. Remove the Power Cartridge and verify that the Eclipse 5 alarms and red Alarm Indicator is flashing and the alarm sounds. After about 5 seconds, re-install the Power Cartridge and connect the AC Adapter and observe that the Eclipse 5 automatically restarts. Confirm that the External Power Present Indicator is illuminated.
9. Turn off Eclipse 5 and unplug the AC Power Supply.
10. Record results, initial and date the Service and Maintenance Record and on service record label located on the machine.
11. EDAT may be utilized to record Eclipse 5 device status and dates of service.

RECORD HOURS OF OPERATION & SOFTWARE VERSION

To help maintain the Eclipse 5, you may obtain the Total Hours of Operation and software version numbers for the Control Board and the Power Manager Systems by following the steps below.

- If connected to the AC or DC Power Supplies, press the “No Smoking” icon on the control panel and advance to the following display mode for each time the icon is depressed:

- Alarm Code (ALRM) - Displays most recent alarm code. Additional alarm codes will also be displayed, if present, by continuing to press the + key.
- Pulse Sensitivity (PS)
- Hours of Operation (HRS)
- 9-volt Battery Status (9V)
- Rise Time (BOL)
- Control Board Software Revision
- Power Manager Software Revision

- If external power is not available and the power cartridge is installed, start by pressing the ON/OFF key for 1 second.

- If no key press is sensed within 5 seconds, the Eclipse 5 will drop out of Provider Mode.

Data Output Form Example

| | |
|---------------------------------------|--|
| Alarm Code | |
| Pulse Sensitivity | |
| Hours of Operation | |
| 9-Volt Battery Status (Volts) | |
| Rise Time | |
| Control Board Software Revision | |
| Power Manager Board Software Revision | |

Log the Results

NOTE:

The display accrues to “99,999” hours, then rolls over to “00,000”.

ELECTRICAL SAFETY TEST

This is required only for the Eclipse 5 Oxygen System, that is used in a hospital or institutional environment. This is not required for home care use.


To test the basic electrical safety of the Eclipse 5 AC Power Supply, CAIRE recommends using an LKG-601 Electrical Safety Analyzer (Netech Corporation, Hicksville, NY) or equivalent to verify that the current leakage to ground is within appropriate limits.

1. Plug the AC Power Supply into the electrical safety analyzer. Disconnect the AC Power Supply from the Eclipse 5 unit.
2. Plug the electrical safety analyzer into a wall outlet.
3. Follow the analyzer manufacturer's instructions for measuring both the forward and reverse earth leakage current only. Verify that forward and reverse-current leakage to ground is $\leq 250 \mu\text{A}$ (100/115VAC applications) and $\leq 500 \mu\text{A}$ (220/240VAC applications).
4. Disconnect the AC Power Supply from the electrical safety analyzer.
5. If the AC Power Supply measures leakage current greater than the criteria in step 3, please return it to CAIRE for service.
6. EDAT may be utilized to record Eclipse 5 device status and dates of service.

CLEANING THE ECLIPSE 5

Clean inside the unit, as needed, using a small vacuum cleaner or brush to remove any accumulation of dust or debris prior to attaching the covers. After reinstalling the cover, verify that the rubber gasket is installed correctly.

Use mild detergent solution to clean the cabinet, Control Panel and power supplies. Turn OFF the Eclipse 5 and disconnect from AC or DC power before any cleaning or disinfection activity. **DO NOT** spray the cabinet Control Panel or power supplies. Use a damp (not soaking wet) cloth or sponge. Spray the cloth or sponge with a mild detergent solution to clean the cabinet and power supplies. To disinfect the Eclipse 5, use Lysol[®] Brand II disinfectant. Proceed as directed by the manufacturer.


| | |
|---|--|
| WARNING: | Unplug Power Cords, AC or DC Power Supplies before cleaning the exterior cabinet. DO NOT use denatured alcohol or apply liquid spray or aerosol cleaners. |
|  | |

SHIPPING AND TRANSPORTING THE ECLIPSE 5

When shipping the Eclipse 5 use original packaging, if possible. Always remove the Power Cartridge and cart from the Eclipse 5 prior to shipping.

If original packaging material is available repack the Eclipse 5, Power Cartridge, cart and power supplies in the designated packaging areas.

If original packaging material is not available, then place the Eclipse 5 in a plastic bag and surround the concentrator with a minimum of two inches of soft foam packing material or bubble wrap. Wrap each accessory in a similar manner. Place the Eclipse 5 and accessories in an appropriate cardboard box for shipping.

| | |
|---|---|
| WARNING: | <u>DO NOT</u> expose the Eclipse 5 to water. The Eclipse 5 enclosure does not provide protection against the harmful effects of liquid ingress. Electrical shock or damage to the unit may result. |
|  | |

When the Eclipse 5 must be transported in a delivery vehicle, simply secure the Eclipse 5 and its accessories to prevent damage. Do not expose the device to extreme heat, cold, or humidity.

STORING THE ECLIPSE 5

Heat and humidity may degrade performance or severely damage the Eclipse 5. Store the device in a cool, dry, protected area away from high temperatures, moisture and humidity. Remove the Power Cartridge when storing the device.

The Eclipse 5 must be turned on and run for 2 hours each month to ensure proper operation performance.

Tip: Running the power cartridge down completely and recharging it will provide two different features for the Eclipse 5:


1. Ensures the battery cartridge is calibrated
2. Running the Eclipse 5 between uses while in storage allows the user to know if service may be needed prior to needing the device.

DISCARDING

Power Cartridge Disposal: The Power Cartridge can be recycled and should not be thrown into the trash. Contact the local city or town offices for instructions on proper disposal of the Power Cartridge. Alternately, CAIRE may be contacted for the Power Cartridge disposal.

Eclipse 5 Oxygen System Disposal: Local environmental laws may prohibit disposal of electrical and/ or electronic equipment such as the Eclipse 5, AC Power Supply or the DC Power Supply. Contact the local city or town offices for instructions on proper disposal of electrical or electronic equipment. Alternately, CAIRE Inc. may be contacted for disposal information.

Troubleshooting, Service, and Repair Procedures

| | |
|---|---|
| CAUTION | The Eclipse 5 contains electrostatic sensitive components. Do not open or handle except at a static free workstation. Do not remove cover without ESD protection. |
|  | |



| | |
|-------|---|
| NOTE: | To adequately troubleshoot and repair the product in the field, EDAT is recommended. Eclipse 5 Data Acquisition Tool (EDAT) PN 5535-SEQ |
|-------|---|

SYSTEM TROUBLESHOOTING AND ALARMS


PROVIDER TROUBLESHOOTING TABLE DO NOT IGNORE ALARMS.

| Yellow Light | | | |
|--|------------|--|--|
| Symptom | Alarm Code | Possible Cause | Provider Action |
| The yellow light is on solid. There is no audible alarm. (This alarm may occur with the Eclipse 5 off while the battery is charging as well) | 001 or 100 | The Eclipse 5 has detected a problem with the connection to the power cartridge. | <ol style="list-style-type: none"> 1) Remove power cartridge and re-install to ensure that it is secure in the concentrator. 2) If possible, install a separate power cartridge in the Eclipse 5 to verify if the condition occurs with multiple batteries. 3) If this problem persists, contact CAIRE Technical Support for service. |
| The yellow light is flashing. The alarm is giving 1 beep every 2 minutes. | 002 | The Eclipse 5 power cartridge is warm. | <ol style="list-style-type: none"> 1) Re-attach the Eclipse 5 to external power or install a fully-charged power cartridge in the Eclipse 5. Allow warm power cartridge to cool outside the concentrator for 30 minutes. 2) Re-charge the power cartridge using AC or DC power. 3) Replace the power cartridge if another is available. 4) If the condition persists, contact CAIRE Technical Support for service. |
| The yellow light is flashing. The alarm is giving 2 beeps every 30 seconds. | 010 | The Eclipse 5 power cartridge voltage is low. | <ol style="list-style-type: none"> 1) Plug Eclipse 5 into AC or DC power supply and recharge or replace power cartridge with fully charged power cartridge. |
| The yellow light is flashing. The alarm is giving 1 beep every 2 minutes. | 020 | The Eclipse 5 has detected a flow restriction causing low or blocked flow. | <ol style="list-style-type: none"> 1) Clean and replace cabinet inlet filter 2) Ensure that the cannula is not kinked or blocked. If used with a humidifier bottle, ensure that it is filled properly and not creating a blockage. 3) Ensure that the Eclipse 5 has proper ventilation. It needs to be at least 3 inches from any surface to ensure the vents aren't blocked. 4) Remove any external tubing attachments to verify that any attached devices are not causing a flow restriction. 5) If the Eclipse 5 has been recently opened for maintenance, verify that no tubing is kinked between the circuit board and the oxygen outlet. 6) If the problem persists, advise patient to switch to alternate source of oxygen and contact CAIRE Technical Support for service. |
| The yellow light is flashing. There is no audible alarm. | 008 | The Eclipse 5 has detected low oxygen levels. | <ol style="list-style-type: none"> 1) Ensure the air intake filter is not clogged or restricted. Clean and replace the filter if necessary. 2) Ensure the Eclipse 5 is in a well ventilated area. Make sure there are at least 3 inches between the back of the Eclipse 5 and any obstructions (furniture, curtain, etc.). 3) If operating in the car, be sure the back of the Eclipse 5 is facing outward in the seat. 4) Perform the preventative maintenance and replace the HEPA, Air Inlet, and Compressor Intake filters. 5) If the condition persists, contact CAIRE Technical Support for service. |

| Red Light (3 LED Models Only) | | | |
|---|------------|---|---|
| Symptom | Alarm Code | Possible Cause | Your Action |
| The red light is flashing. The alarm is giving 3 beeps every 2 minutes. | 004 | The Eclipse 5 has detected low oxygen levels | <ol style="list-style-type: none"> 1) Ensure the air intake filter is not clogged or restricted. Clean and replace the filter if necessary. 2) Ensure the Eclipse 5 is in a well ventilated area. Make sure there are at least 3 inches between the back of the Eclipse 5 and any obstructions (furniture, curtain, etc.) 3) If operating in the car, be sure the back of the Eclipse 5 is facing outward in the seat. 4) Verify that the internal filters (HEPA, Compressor Intake) are clean and not restricted. If necessary, replace filters. 5) If the condition persists, advise patient switch to an alternate source of oxygen and contact CAIRE Technical Support for service. |
| The red light is solid. The alarm is giving a constant beep. The Eclipse 5 is not delivering oxygen and it will not power on. | “*****” | The Eclipse 5 has lost power temporarily while running on external power and needs to be re-set. | <ol style="list-style-type: none"> 1) Remove the power cartridge and disconnect the AC or DC power supply from the Eclipse 5. The red light should disappear when the power sources are removed. Wait approximately 20 seconds, reconnect power sources, and attempt to power on the Eclipse 5 again. If the Eclipse 5 does not power on, proceed to step 2. 2) Inspect the external (AC or DC) power supply and ensure that its connections are secure at the Eclipse 5, the transformer, and the external power outlet. 3) If possible, attempt to use another electrical (AC or DC) outlet to power the Eclipse 5. 4) Verify that the status LED on the external power supply (AC or DC) and external power LED on the Eclipse 5 are lit. If they are not, attempt to use another external (AC or DC) power supply to see if the problem persists. 5) If the condition persists, contact CAIRE Technical Support for service. |
| | N/A | The Eclipse 5 has lost power due to a depleted power cartridge charge or an overheated power cartridge. | <ol style="list-style-type: none"> 1) Reset the Eclipse 5 by removing the power cartridge and external (AC or DC) power supply. 2) Re-attach the Eclipse 5 to external power or install a fully-charged power cartridge in the Eclipse 5. Allow warm power cartridge to cool outside the concentrator for 30 minutes. 3) Re-charge the power cartridge using AC or DC power. 4) Replace the power cartridge if another is available. 5) If the condition persists, contact CAIRE Technical Support for service. |
| The red light is solid. The display screen says “FAIL”. The Eclipse 5 is not producing delivering oxygen and will not power on. | FAIL XX | The Eclipse 5 has experienced a system malfunction. | <ol style="list-style-type: none"> 1) Remove the power cartridge and disconnect the AC or DC power supply from the Eclipse 5. The red light should disappear and the FAIL message will disappear from the screen when the power sources are removed. Wait approximately 20 seconds, reconnect power sources, and attempt to power on the Eclipse 5 again. 2) If the Eclipse 5 does power on, monitor it to determine if the FAIL message occurs again. If the FAIL message occurs again, contact CAIRE technical support for service. 3) If the Eclipse 5 does not power back on, advise patient switch to an alternate source of oxygen and contact CAIRE Technical Support for service. |

| Other Alarm Conditions | | | |
|--|------------|--|---|
| Symptom | Alarm Code | Possible Cause | Your Action |
| While in pulse mode, the compressor speeds up and the pulse mode LED flashes quickly for 15 seconds. | N/A | The Eclipse 5 is unable to detect the user’s breathing effort. See page 17 for pulse mode information. | <ol style="list-style-type: none"> 1) Pulse mode may not work correctly if the user has any condition that causes blocked/restricted nasal passages (Illness, deviated septum, etc.). Switch to continuous flow. 2) Ensure cannula is no longer than 7 feet in length. 3) Ensure that there are no kinks or blockage in cannula tubing. 4) If a humidifier bottle is connected, remove the humidifier bottle and connect cannula directly to outlet port. Note: Pulse mode will not work with a humidifier bottle installed. 5) If the condition persists, contact CAIRE Technical Support for service. |

| Other Alarm Conditions (Continued) | | | |
|---|------------|--|--|
| Symptom | Alarm Code | Possible Cause | Your Action |
| Power Cartridge is draining while plugged in to AC/DC power supply | N/A | The Eclipse 5 is not receiving power from the attached power supply. | <ol style="list-style-type: none"> 1) Verify that the outlet is providing power. Do not connect the power supply to a dimmer circuit or a power strip. 2) Check that cable connections on power supplies are secure to the wall/vehicle and concentrator. If using the AC or DC power supply, check the cable connection on the power supply transformer as well. 3) Ensure that the power verification lights are on. <ul style="list-style-type: none"> - There will be a green light on the power supply transformer box. - There will be a green light on the Eclipse 5 concentrator control panel in the shape of a power cord. 4) If power verification LEDs are not lit, remove all connections of the power supply for 20 seconds and reconnect. 5) If the condition persists, contact CAIRE Technical Support for service. |
| The Power Cartridge (battery) charge is not lasting as long as it should. | N/A | The power cartridge was not fully charged | <ol style="list-style-type: none"> 1) Connect to AC or DC power to recharge the battery. Verify that the battery charges for 2-5 hours and the battery icon is full and not flashing before use. 2) Refer to the actions for "Power Cartridge is Not Charging" Symptom below. |
| | | The Eclipse 5 was not operating at the anticipated flow rate. | <ol style="list-style-type: none"> 1) Ensure that the prescribed flow rate is being used and that pulse or continuous flow is being used as required. |
| | | The power cartridge is not performing to specifications. | <ol style="list-style-type: none"> 1) Attempt to drain the battery cartridge completely. Do this by running the Eclipse 5 on battery power until the machine shuts off completely. Then remove the battery and allow it to cool for approximately 30 minutes. After this time, re-insert the battery in the Eclipse 5 and recharge it using AC or DC power. Perform the Battery Calibration procedure on page 36. 2) Time the battery duration and compare it to the chart on page 22. 3) If the battery duration is less than 80% of the run time listed in the chart on page 22 after the battery calibration, it is recommended to replace power cartridge. |
| The Power Cartridge (battery) is not charging. | N/A | The Eclipse 5 is not receiving external AC or DC power to charge the battery. | <ol style="list-style-type: none"> 1) Verify that the outlet is providing power. Do not connect the power supply to a dimmer circuit or a power strip if using AC power supply. 2) Check that cable connections on power supplies are secure to the wall/vehicle and concentrator. If using the AC power supply, check the cable connection on the power supply transformer as well. 3) Ensure that the power verification lights are on. <ul style="list-style-type: none"> - There will be a green light on the power supply transformer box. - There will be a green light on the Eclipse 5 concentrator control panel in the shape of a power cord. 4) If power verification LEDs are not lit, remove all connections of the power supply for 20 seconds and reconnect. 5) If the condition persists, contact CAIRE Technical Support for service. |
| | N/A | The Eclipse 5 is not properly communicating with the power cartridge to charge it. | <ol style="list-style-type: none"> 1) Remove power cartridge and re-install to ensure that it is secure in the concentrator. 2) Inspect the Eclipse 5 for a solid yellow light when the battery is installed or a flashing battery icon when attempting to charge. If either of these symptoms is present, continue to step 3. 3) If possible, install a separate power cartridge in the Eclipse 5. If the replacement cartridge works properly, then the original cartridge needs to be replaced. 4) If this condition persists, contact CAIRE Technical Support for service. |
| The Eclipse 5 beeps 3 times when it is first powered on. | N/A | The internal battery that powers the alarms is low | Internal 9V battery needs replacement. Perform preventative maintenance or contact CAIRE Technical Support for service. |

| | |
|---|---|
| WARNING: | WARNING: Do not modify this equipment without authorization of the manufacturer. |
|  | |

ALARM CONDITIONS AND ALARM CODES

Use the table below to decode Eclipse 5 alarm conditions. If other alarm codes are displayed by the Eclipse 5, contact CAIRE Technical Support for assistance.

Note: The following table is intended as a guide for the provider, not the user. 3 LED units:

| CONDITION | ALARM CODE | ALARM DISPLAY | GREEN INDICATOR | YELLOW INDICATOR | RED INDICATOR | AUDIBLE ALARM | WHAT TO DO |
|--|------------|------------------|-----------------|------------------|---------------|---------------------------|--|
| "Warming Up. Please Wait." | 004 | O2 < 70% | ON | ON | ON | OFF | Wait. The system typically takes 3 – 5 minutes to reach specified performance. |
| "Warming Up. Please Wait." | 008 | O2 < 85% | ON | ON | OFF | OFF | Wait. The system typically takes 3 – 5 minutes to reach specified performance. |
| "3.0"(or flow setting) | 000 | NO ALARM | ON | OFF | OFF | OFF | Nothing. The system is operating properly at the specified flow rate. |
| "Low Power Cartridge" | 010 | LOW BAT | ON | Flashing | OFF | 2 Beeps | Plug into external power or replace with a charged Power Cartridge. |
| "Warm Power Cartridge" | 002 | WARM BAT | ON | Flashing | OFF | 1 Beep | Plug into external power or replace with a charged Power Cartridge. |
| "Low 9V Battery" | - | - | OFF | OFF | OFF | 3 Beeps on POST | Replace the internal 9-volt battery. |
| "O ₂ Concentration < 85%" | 008 | O2 < 85% | OFF | Flashing | OFF | OFF | Perform Annual Filter PM Maintenance. If condition persists, service is required. |
| "O ₂ Concentration < 70%" | 004 | O2 < 70% | OFF | OFF | Flashing | 3 Beeps | Perform Annual Filter PM Maintenance. If condition persists, service is required. |
| "Flow Rate Error / Blocked Flow" | 020 | FLOWRATE | OFF | Flashing | OFF | 1 Beep | Check tubing and/or humidifier for obstruction. Check/clean air intake filter. If condition persists past 10 minutes, service is required. |
| "Cannot Charge Power Cartridge" | 001 | CHARGER | N/A | ON | OFF | OFF | Instruct patient to seek an external power source. Remove Power Cartridge and allow to cool to room temperature. If Power Cartridge malfunction persists, service is required. |
| "One Wire Communication Loss" | 100 | ONEWIRE | N/A | Flashing | OFF | 1 Beep | Check battery connections. |
| "No Inspiration Detected" (in Pulse Mode only) | 200 | P <-> C | ON | OFF | OFF | OFF | If no inspiratory effort is detected after 15 seconds, the Eclipse 5 will switch to Continuous Flow for 15 seconds, and continue this sequence until a breath is detected. |
| "Loss of External Power" (without charged Power Cartridge installed) | 040 | ***** (flashing) | OFF | OFF | Flashing | ON for 5 min | Instruct patient to seek an alternative oxygen supply until external power is restored or install a charged Power Cartridge. |
| "System Fault" | 080 | FAIL XX | OFF | OFF | ON | ON 10 seconds then silent | Reset power, wait 20 seconds, reconnect power, restart device. Instruct patient to use back up oxygen supply. Service is required. |

Alarms Table

2 LED units

| Alarm | LCD Text | Green | Yellow | Audio | Code |
|---|-----------|-----------------|--------|---|------|
| All OK, warm-up done | NO ALARM | ON | OFF | OFF | 000 |
| Warm-up O2 < 85% | O2 LOW | ON | ON | No Beeps | 008 |
| No breath detected (less than 45 seconds) | NO ALARM | ON | OFF | OFF | 000 |
| No breath detected (exceeding 45 seconds) | P <--> C | ON | ON | 1 alarm beep, repeat every 20 seconds | 200 |
| One wire communication loss | ONE WIRE | ON OR OFF | ON | 1 alarm beep, repeat every 20 seconds | 100 |
| Cannot charge battery | CHARGER | ON OR OFF | ON | 1 alarm beep, repeat every 20 seconds | 001 |
| Ambient pressure fail | AMB PRESS | ON OR OFF | ON | 1 alarm beep, repeat every 20 seconds | 004 |
| O2 < 85% (After warm-up) | O2 LOW | OFF | ON | 1 alarm beep, repeat every 20 seconds | 008 |
| Flow rate error > +/-10% | FLOWRATE | OFF | ON | 1 alarm beep, repeat every 20 seconds | 020 |
| Warm battery > 60°C | WARM BAT | ON | ON | 1 alarm beep, repeat every 20 seconds | 002 |
| Low battery | LOW BAT | ON | ON | 1 alarm beep, repeat every 20 seconds | 010 |
| Loss of power | ***** | OFF | ON | 1 alarm beep, repeat every 20 seconds for 200 seconds | 040 |
| Malfunction | FAIL XX | OFF | ON | 1 alarm beep, repeat every 20 seconds for 200 seconds | 080 |

MALFUNCTION CODES

If a malfunction occurs in the Eclipse 5, the device will stop, the Red LED on the front panel will light and the buzzer will sound for 10 seconds and then silence. The LCD will display one of the following Malfunction Codes:

| Malfunction | FAIL code | Recommended Action |
|------------------------------------|-----------|--|
| Invalid RESET | FAIL 80 | Check for secure communication cables, Verify functionality of PM and CS PCBs |
| I/O Port Failure | FAIL 81 | Check for secure communication cables, Verify functionality of PM and CS PCBs |
| RAM Failure | FAIL 82 | Check for secure communication cables, Verify functionality of PM and CS PCBs |
| FLASH Failure | FAIL 83 | Check for secure communication cables, Verify functionality of PM and CS PCBs |
| EEPROM Failure | FAIL 84 | Check for secure communication cables, Verify functionality of PM and CS PCBs |
| IPC Watchdog Timeout | FAIL 90 | Check for secure communication cables, Verify functionality of PM and CS PCBs |
| Compressor Motor Too Hot | FAIL 91 | Allow Eclipse 5 to Cool for 30 Minutes. Check compressor fan functionality. Check to ensure vents are not obstructed. Verify functionality of the Compressor Assy |
| PCB Too Hot | FAIL 92 | Allow Eclipse 5 to cool for 30 Minutes. Verify functionality of PM fan. Check to ensure vents are not obstructed |
| Compressor Motor Stalled | FAIL 94 | Check Compressor wires for damage. Verify functionality of PM PCB. Verify functionality of the Compressor Assy |
| Battery Communication Failure | FAIL 95 | Verify functionality of the Battery Bridge PCB. Check Battery and Battery Bridge PCB for pin damage. Verify functionality of battery. Verify functionality of PM pcb |
| IPC Failure | FAIL A0 | Verify functionality of PM PCB |
| Product Pressure Sensor Failure | FAIL A1 | Verify functionality of CS PCB |
| Breath Pressure Sensor Failure | FAIL A2 | Verify functionality of CS PCB |
| Ultrasonic Failure | FAIL A3 | Verify functionality of CS PCB. Check for water intrusion from humidifier |
| Product Temperature Sensor Failure | FAIL A4 | Verify functionality of DB9 cable harness. Verify functionality of CS PCB |
| Loss of Product Tank Pressure | FAIL A5 | Check for leaking, cracked HEPA filter or damaged tubing. Verify ATF motor is turning |
| Purity Calibration Data Failure | FAIL A6 | Check for leaking, cracked HEPA filter or damaged tubing. Verify functionality of CS PCB |
| Flow Calibration Data Failure | FAIL A7 | Verify functionality of Proportional Valve. Verify functionality of CS PCB |
| Breath Sensitivity Data Failure | FAIL A8 | Check for damaged tubing. Verify functionality of CS PCB |
| Hour of Operation Data Failure | FAIL A9 | Verify functionality of CS PCB |
| Invalid Assembly Option | FAIL AA | Remove Power to Reset |
| Ambient Pressure Sensor Failure | FAIL AB | Verify functionality of CS PCB |
| Unidentified Failure | FAIL FF | Remove Power to Reset |

Step 1: Remove all power sources; battery and external power. Wait 20 seconds. Reconnect power to the Eclipse 5. Turn the device to the ON position. If resolved, continue use.

Step 2: If unresolved, call CAIRE Technical Support for assistance.

System Schematics and Diagrams

SIMPLIFIED BLOCK DIAGRAM

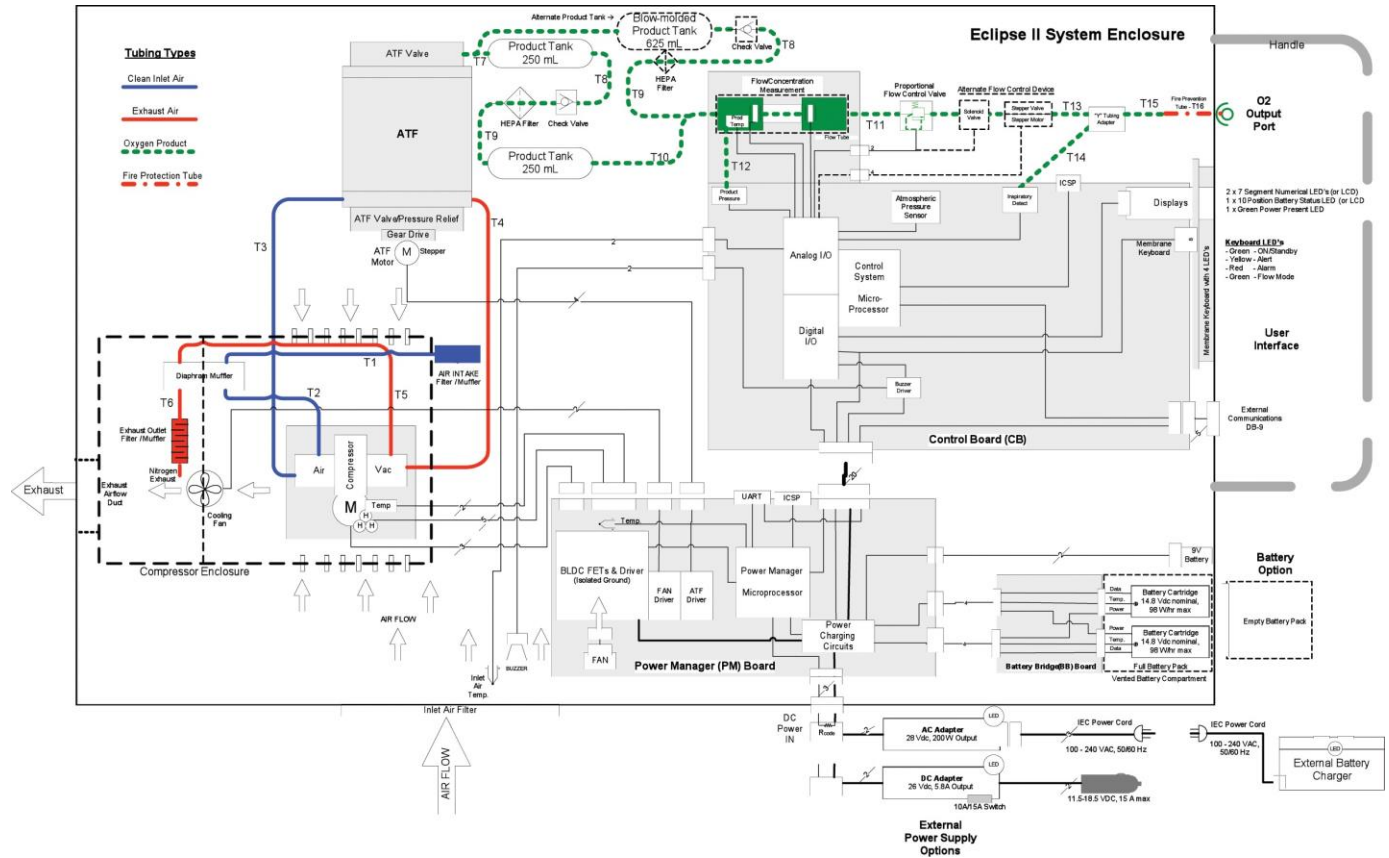


Figure 28: Eclipse 5 Oxygen System Simplified Block Diagram.

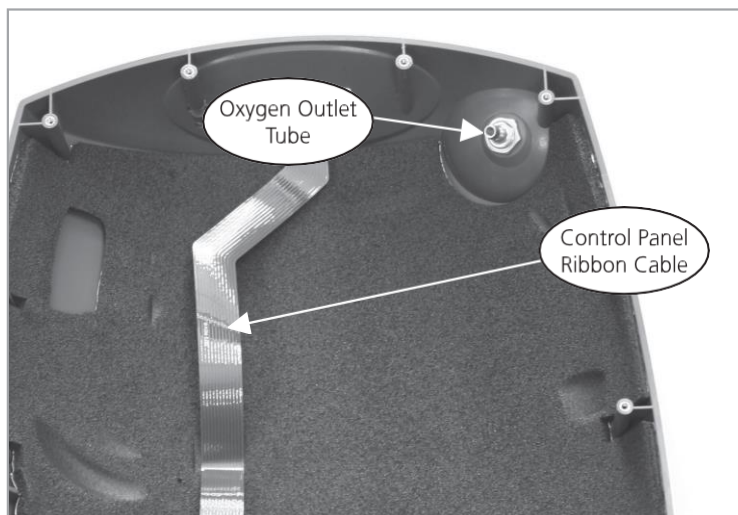


Figure 29: Top Case Components.

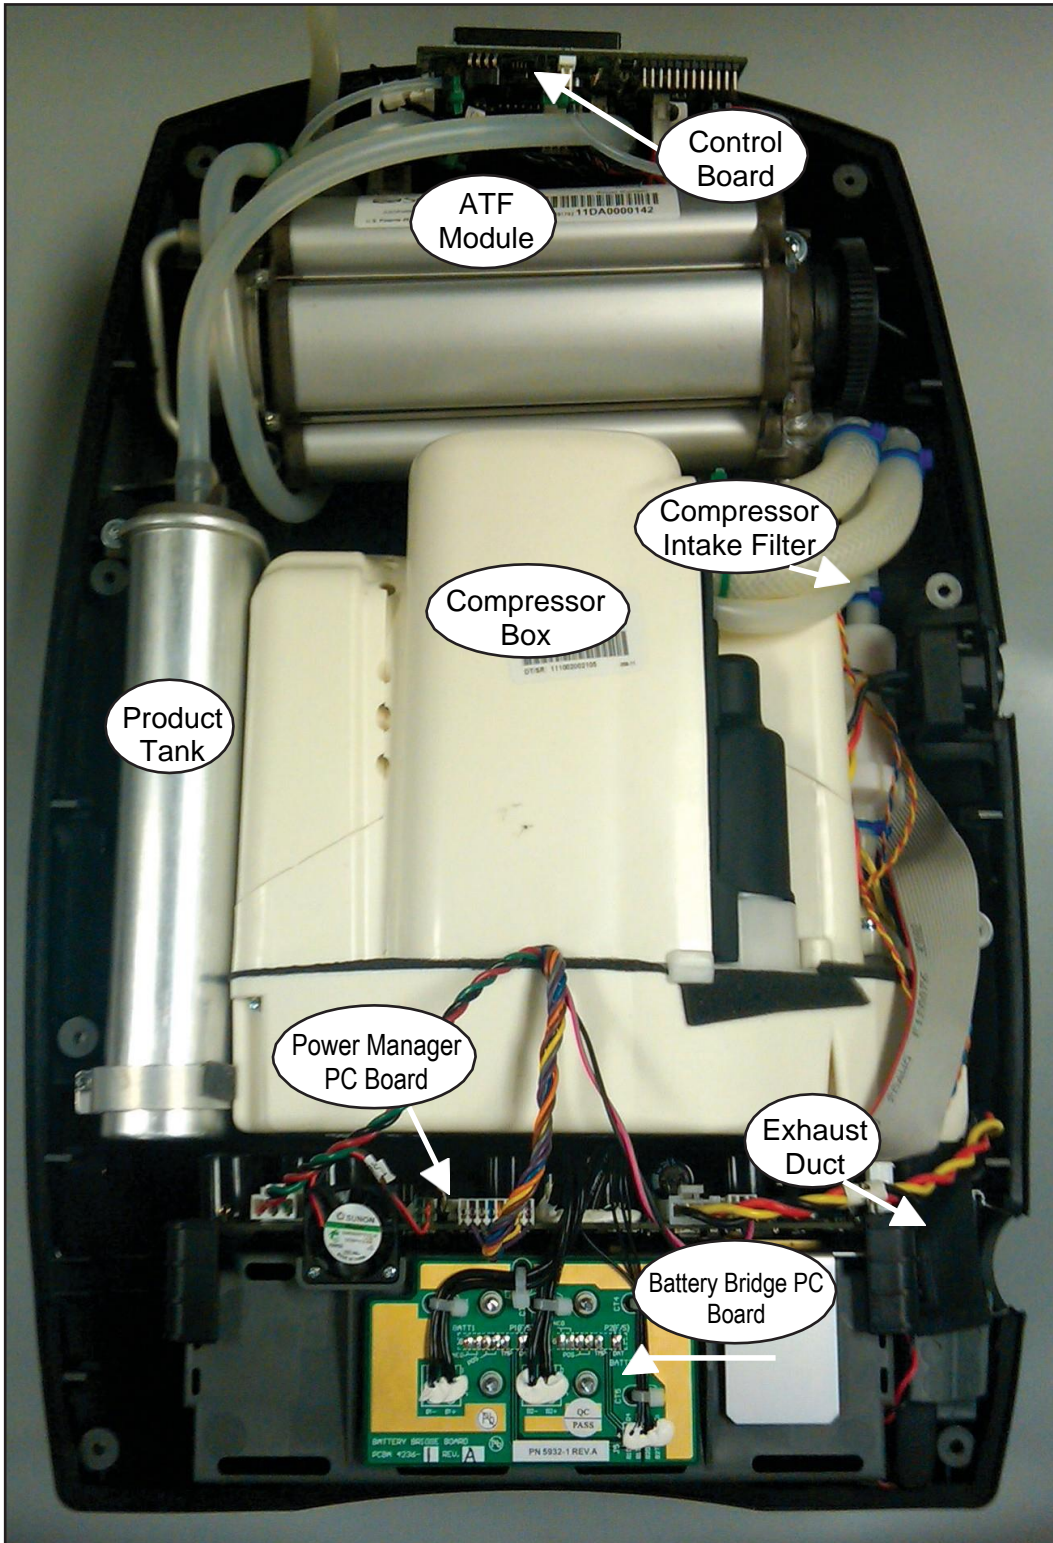


Figure 30: Bottom Case Components

Oxygen Circuit

REMOVE AND REPLACE THE ATF MODULE

NOTE:

There are no serviceable parts inside the ATF Module. Do not attempt to disassemble or modify the ATF Module.

1. Remove the Unit Cover as described in the section Remove and Replace the Unit Cover.
2. Cut the cable tie as shown below, and disconnect the silicone tube that goes into the product port of the ATF; this tube comes from the Product Tank.
3. Install port cap.

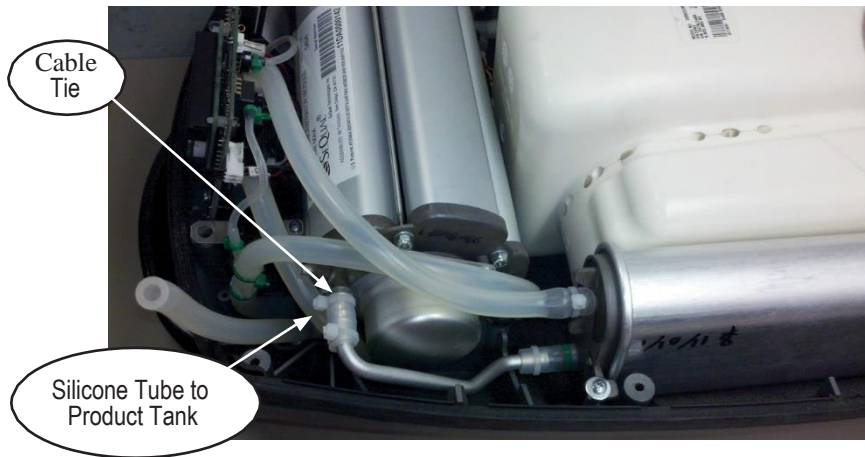


Figure 31: Removal of ATF Module Product Hose.

4. Cut the cable tie that secures the silicone tube to the braid tube at shown below.

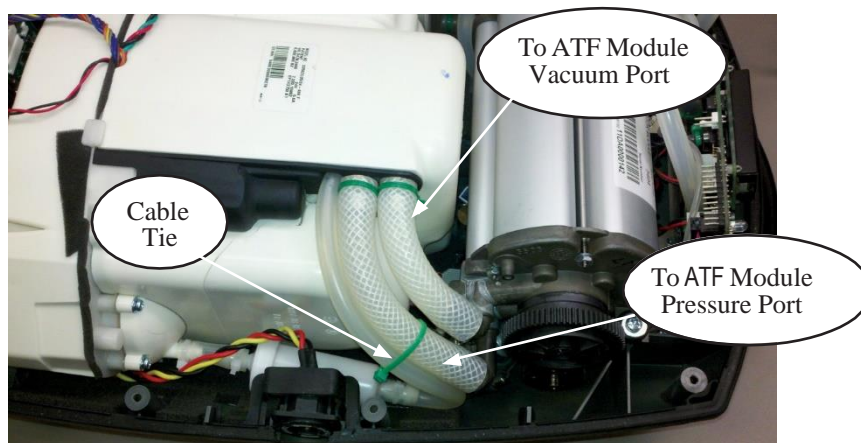


Figure 32: Removal of ATF Module Pressure and Vacuum Tubes.

5. Cut the cable ties to the braided tubes that connect into the ATF pressure and vacuum ports as shown in Figure 32. Disconnect the braided tubes.
 - 5a. Install port caps.
6. Unscrew the 3 screws (M4x16 Pan Head Machine Screw, P/N 6961-416-SEQ) and remove the screws and washers (M4 Flat washer, P/N 6985-04-SEQ) as shown below.

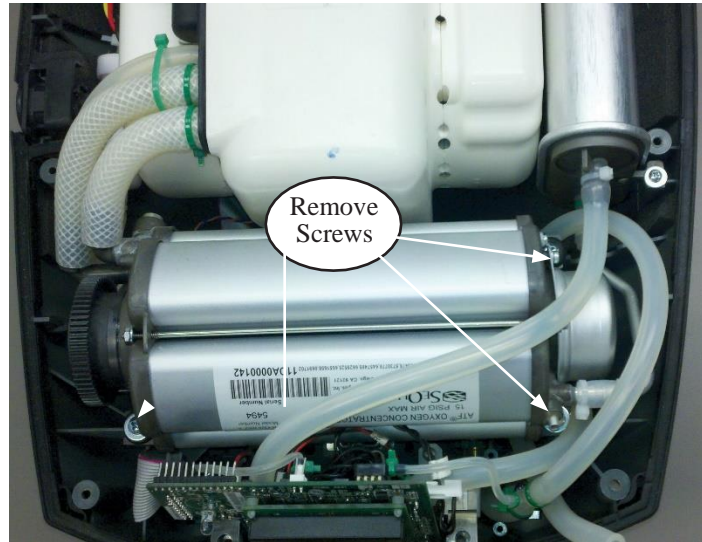


Figure 33: Remove ATF Module from Eclipse 5 Case.

7. Lift the ATF. Take off the 3 grommets. Disconnect the wire harness from the gearbox of the ATF.
8. Remove the ATF.
9. Install 3 grommets into the mounting slots on the ATF as shown below. Position the ATF into the bottom cover but DO NOT install the mounting screws yet. Route the 16" Silicone Tube under the ATF as shown on Figure 35 on next page.



Figure 34: ATF Module Grommet Installation

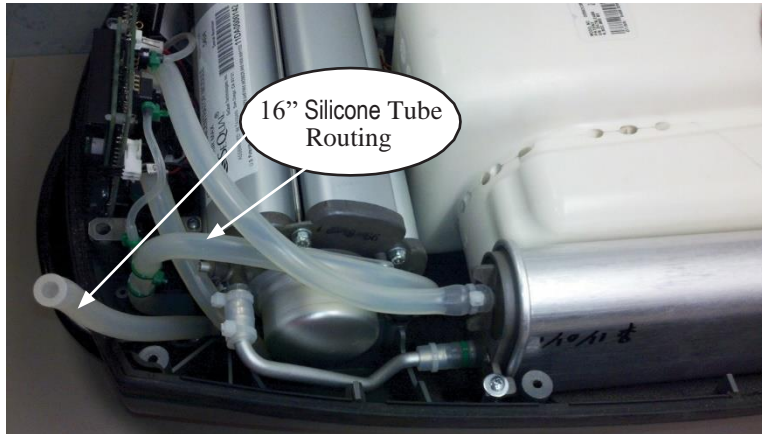




Figure 35: Tube Routing under ATF Module.

- Place the ATF in the Unit Case and remove the caps from the ATF Ports. Install the Braided Tubes into the ATF pressure and vacuum ports as shown on Figure 32. Do not use oil or grease if the tubing is difficult to install. Secure joints with cable ties.

| | | |
|-----------------|--|---|
| WARNING: |  | DO NOT use any petroleum based or other lubricants. A spontaneous and violent ignition may occur if oil, grease or other petroleum substances come into contact with oxygen under pressure. Keep these substances away from the oxygen system, tubing and connections and any other oxygen source. |
| NOTE: | | Inspect all tubing before securing with a cable tie. |

- Mount the ATF with 3 M4x16 screws and 3 washers as shown on Figure 33 on previous page. Apply Loctite® 425 Thread Locker on the threaded tips of the screws before installing. Tighten screws but **DO NOT** squash the grommets (2 in.lbs. maximum).

If needed, install spacer (20623336) underneath the ATF mount closest to the product tank with a longer screw (6961-418-SEQ) to ensure that the ATF is level.

| | |
|---|--|
| NOTE: | Over tightening may cause excess vibration. |
| CAUTION | Remove caps on ATF ports ONLY before connecting the tubes. DO NOT leave the ports open unless ready to install the tubes. Also place the removed caps from the new ATF and place on the ports of the replaced ATF. |
|  | |

12. Remove caps from ATF Module.
13. Connect the silicone tube from the Product Tank into the product port of the ATF and secure joints with cable ties as shown on Figure 31.
14. Use cable tie to secure the silicone tube to the braid tube to ensure that there is NO kinking on the bend as shown on Figure 32. Hand-tighten the cable tie. Inspect the tubing to ensure the tubing is not kinked.
15. Perform product test prior to installing cover and again after cover replacement.
16. Installation of the Unit Cover on the unit is described in the Remove and Replace of the Unit Cover.

REMOVE AND REPLACE THE PRODUCT TANK ASSEMBLY (PN 4378-SEQ)

Removal of Product Tank

- 1) Follow the steps to Removing the Unit Cover
- 2) Remove the Front Cover Assembly completely; disconnect outlet tubing and front membrane ribbon cable. Set aside.
- 3) Locate the Product Tank and cut the cable ties from the ATF to the product tank (Bottom), and O2 out from the outlet connector (Top). Remove tubing from ATF to lower product tank barb. See Figure 36.

Important: Cap off the ATF hose barb with a black hose barb cap.



Figure 36: Cut Cable Ties

- 4) Locate the 2 screws that hold the securing straps and the product tank in place, remove the screws. Set aside for re- installation. Figure 37.



Figure 37: Remove Screws

- 5) Lift out the old product tank. Set aside for RMA return or scrap.

Install new Product Tank

1) Locate all parts needed: Product Tank, Product Tube from ATF (correct version), Securing arm and screws. See Figure 38.




Figure 38: New product tank

2) Position the product tank with the 2 hose barbs facing in the direction of the ATF. Refer to Figure 39.



Figure 39: Product tank and hose barbs

- 3) Install the securing arm over the product tank, and locate the screw hole on the back case cover to secure the product tank.

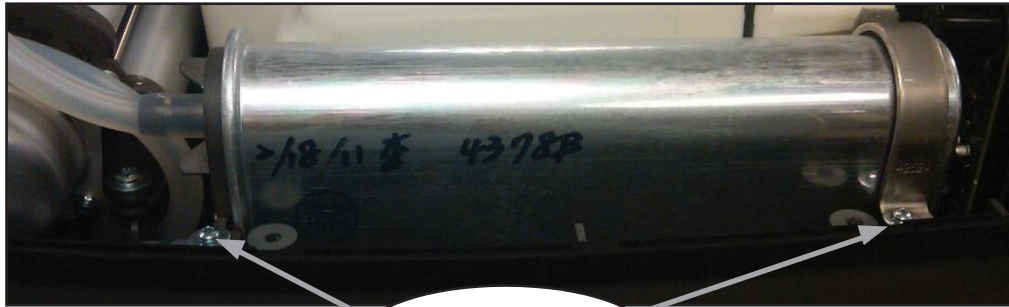

Install securing arm
and install two screws

Figure 40: Install securing arms

- 4) Locate the correct Product Tube - remove black ATF outlet barb cap, and attach the Product Tube Assy to the ATF output barb, secure with a cable tie. Attach the other end of the Product Tube to the Bottom port on the Product Tank. See Figure 39.
- 5) Connect the Output tubing to the Top port on the Product Tank and secure with cable ties. See Figure 41.




Add cable tie to both
top and bottom parts

Figure 41: Connect output tubing

Electronics

REMOVE AND REPLACE THE CONTROL BOARD ASSEMBLY

| | |
|---|---|
| CAUTION | The Eclipse 5 contains electrostatic sensitive components. Do not open or handle except at a static free workstation. |
|  | |

| | |
|--------------|---|
| NOTE: | The Control Board Assembly is factory calibrated as a single unit. Do not disassemble the Control Board Assembly. |
|--------------|---|

1. Remove the Unit Cover as described in the section Remove and Replace the Unit Cover.

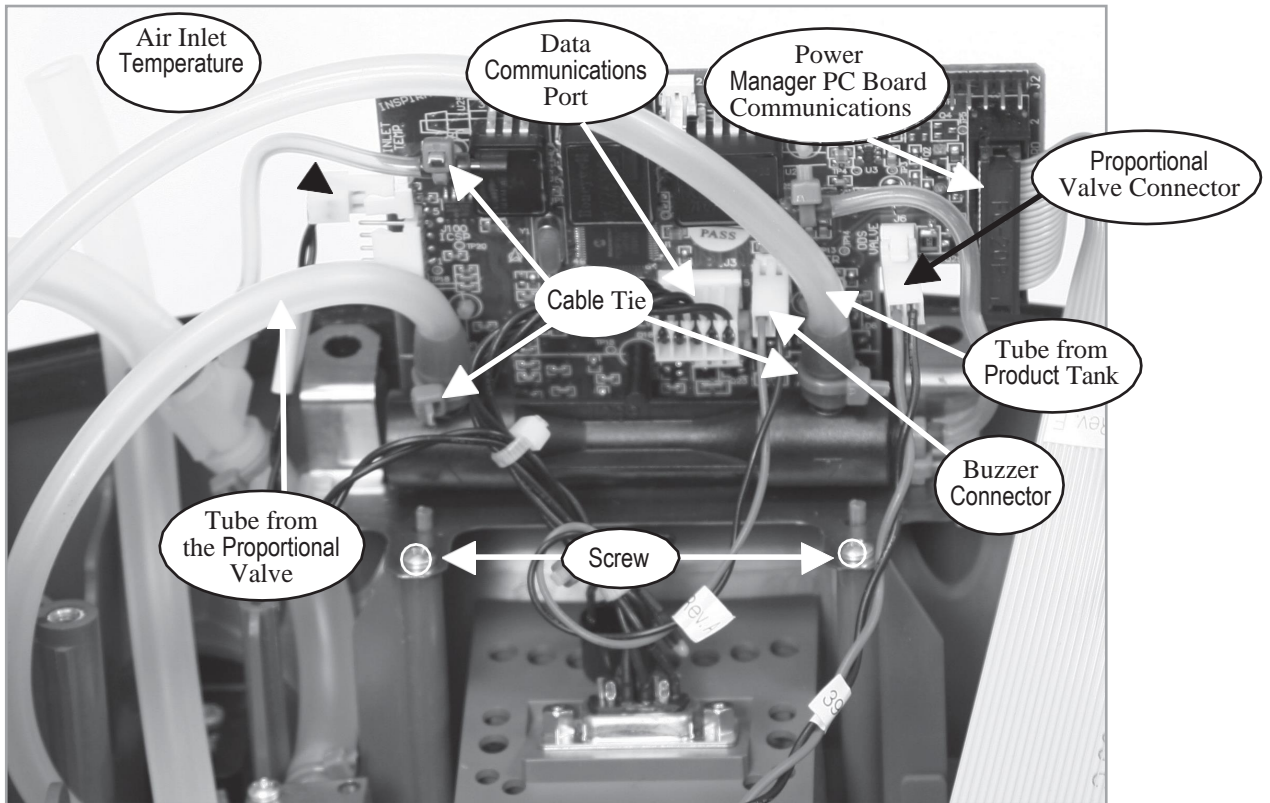


Figure 42: Control Board Removal (ATF Module not shown for clarity).

2. Remove the 2 screws (M3x10 Plastic Screw, P/N 6950-310-SEQ) holding the Control Board Assembly to the Unit Case as shown in Figure 42.

| | |
|--------------|---|
| NOTE: | Use a magnetized Phillips #1 screwdriver to remove the screws. This greatly reduces the chances of dropping a screw in the Unit Case. |
|--------------|---|

3. Lift the Control Board Assembly and disconnect the Inlet Air Temperature, Data Communications Port, Power Manager PC Board Communications, Proportional Valve wire harness, and Buzzer wire harnesses as shown in Figure 42.

4. Lift the Control Board out of the Unit. Cut the green cable tie to the silicone tube that is connected to the sensor as shown in Figure 42. Disconnect the silicone tube that is attached to the sensor. Cut the green cable ties to the silicone tubes that are connected to the flow tube as shown in Figure 42. Disconnect the silicone tubes that are attached to the flow tube.
5. Pinch or plug the silicone tube coming from the ATF product port and secure with a cable tie.
6. Remove the Control Board Assembly.
7. To install a new Control Board Assembly, cut the cable tie used to pinch the silicone tube coming from the product tank. Attach this tube and the tubes from the Proportional Valve and from the Product Tank to the flow tube as shown in Figure 42. Secure with a cable tie. Connect the silicone tube to the sensor as shown in Figure 42. Secure with a cable tie. Place the 2 screws in the sheet metal bracket as shown in Figure 43. Inspect the tubing to ensure the tubing is not kinked.
8. Lower the Control Board Assembly into the Unit Case only to where the aligning pins go through the sheet metal bracket; make sure the sheet metal bracket is 1/8" above the supporting ribs – this will ensure the 2 screws stay in the bracket and do not fall in the unit case as shown in Figure 43. Start the 2 screws by turning them 2 times into the unit case. After starting both screws, lower the Control Board Assembly onto the supporting ribs; tighten the 2 screws to the unit case.

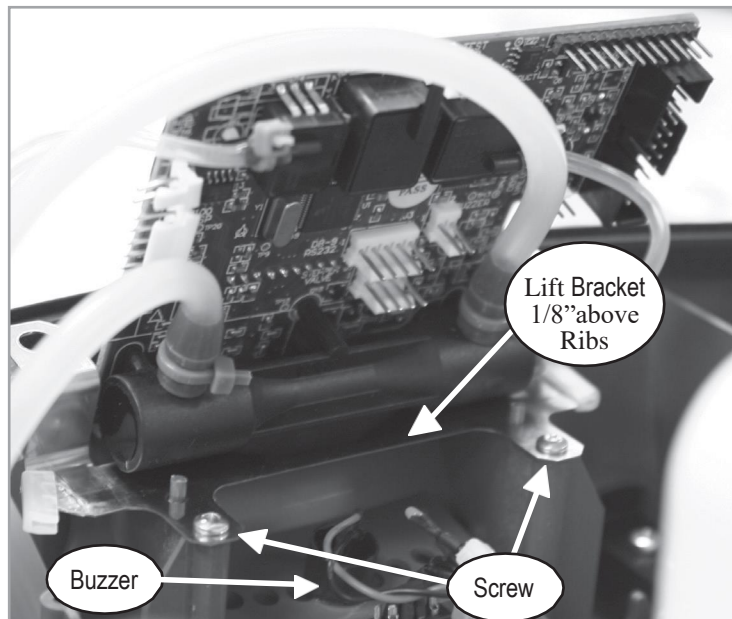


Figure 43: Control Board Installation.

9. Connect the Inlet Air Temperature, Data Communications Port, Power Manager PC Board Communications, Proportional Valve wire harness and Buzzer wire (3 LED model), or Speaker wire (2 LED model) harnesses as shown on Figure 42.
10. Refer to “Flow Calibration” in EDAT User Manual (PN 5419-SEQ) to calibrate Eclipse 5 with new Control Board.
11. Installation of the unit cover on the unit is described in the Remove and Replace of the Unit Cover.
12. Add serial number scanner T-10496 to write Eclipse S/N to EPROM, Instructions found in CMI-028.

REMOVE AND REPLACE THE BUZZER WIRE HARNESS (3 LED model)

1. Unplug the buzzer from the Control Board PC Board.
2. Remove the Control Board.
3. To remove the buzzer from the case, cut the cable tie, grasp the buzzer body with a pair of pliers and rotate the buzzer to break the adhesive joint.
4. To install a new buzzer, apply a ring of cyanoacrylate adhesive (Super Glue) around the inlet hole as shown in Figure 44.
5. Place buzzer as shown in Figure 44. Ensure that the buzzer opening is centered over the grill hole. Hold in place until adhesive cures.

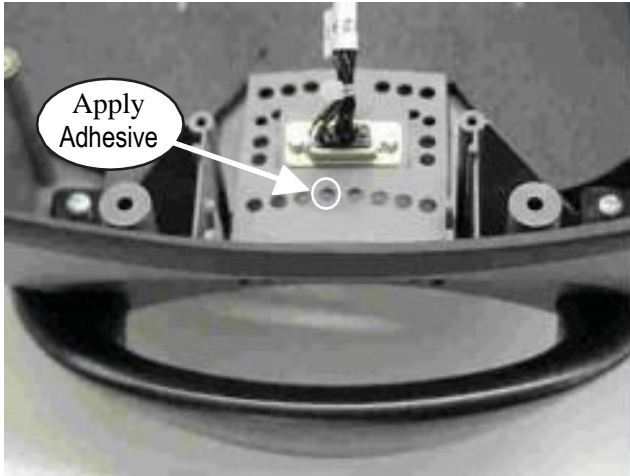


Figure 44: Bonding the Buzzer to the case.

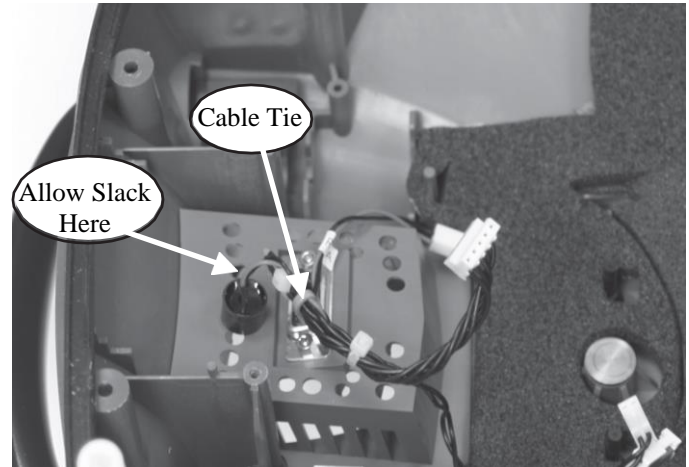


Figure 45: Buzzer Installation.

6. Install the Control Board Assembly. Secure the wire harness with Cable as shown on Figure 45. Insure that there is slack on the wire harness before tightening the Cable Tie. Plug in the buzzer.

REMOVE AND REPLACE THE SPEAKER WIRE HARNESS (2 LED model)

1. Unplug the speaker from the Control Board.
2. To remove the speaker from the case, remove 2 screws.
3. To install a new speaker, use 2 screws as shown on Figure 45b.

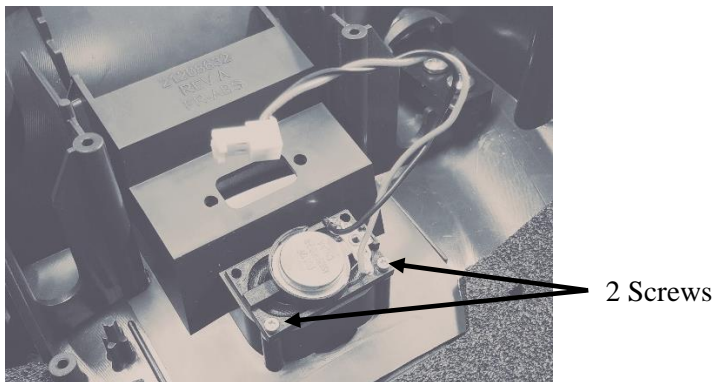


Figure 45b: Speaker Installation.

4. Plug the speaker cable into Control Board Assembly.

CONTROL BOARD CONNECTOR DIAGRAM

Use the figure below as an aid to ensure proper connection of wire harnesses to the Control System printed circuit board.

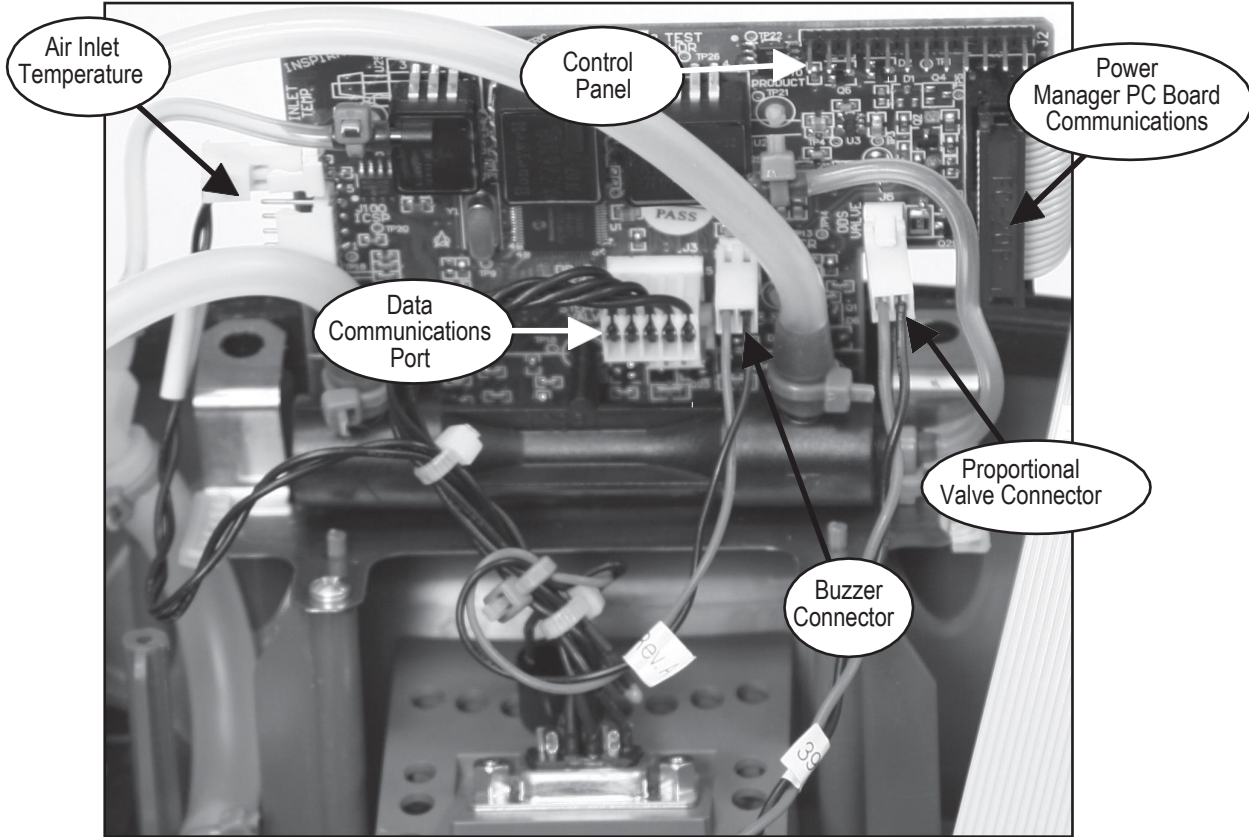


Figure 46a: Control Board Connector Diagram 3 LED Model

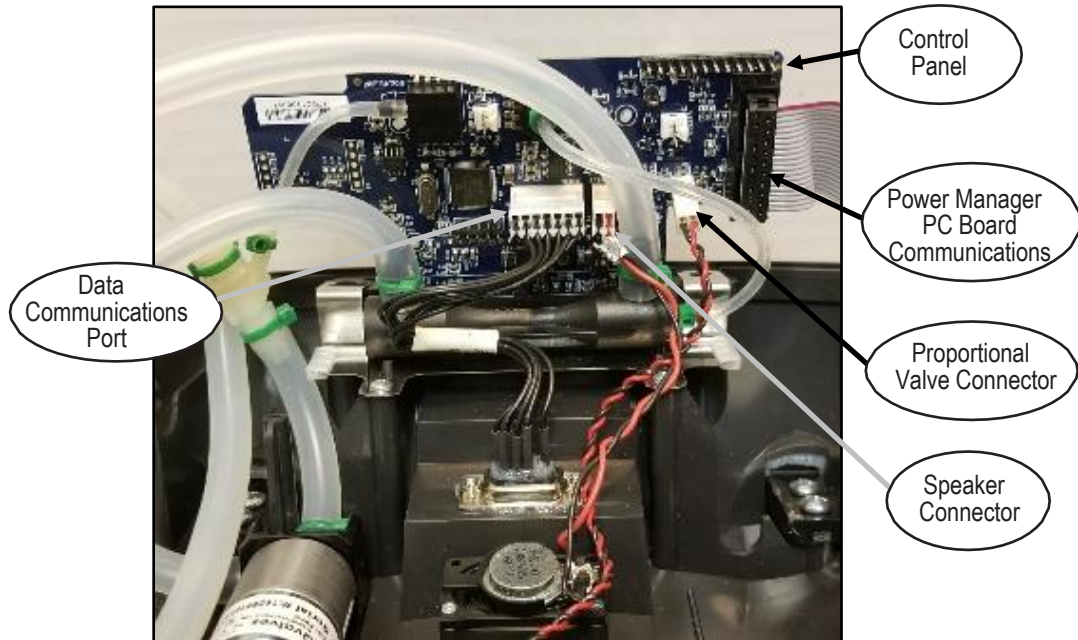




Figure 46b: Control Board Connector Diagram 2 LED Model

Remove and Replace Power Manager Printed Circuit Board

1 Remove and Replace Combo Power Manager board set

| | |
|---|--|
| WARNING: | <p>Disconnect power supplies and remove Power Cartridge before removing the unit cover. Do not touch exposed circuits during maintenance without ESD protection.</p> |
|  | |
| CAUTION | <p>The Eclipse 5 contains electrostatic sensitive components. Do not open or handle except at a static free workstation.</p> |
|  | |

1.1 Remove the Power Cartridge and unscrew the 4 screws (PN: 6974-312-SEQ) holding the BBB pcb to the case shown in Fig 47.



Fig 47: Screws

1.2 Remove the Unit cover as described in section, “Remove and Replace the Unit Cover”.

1.3 Disconnect the 5 wire harnesses as shown in Figure 48.

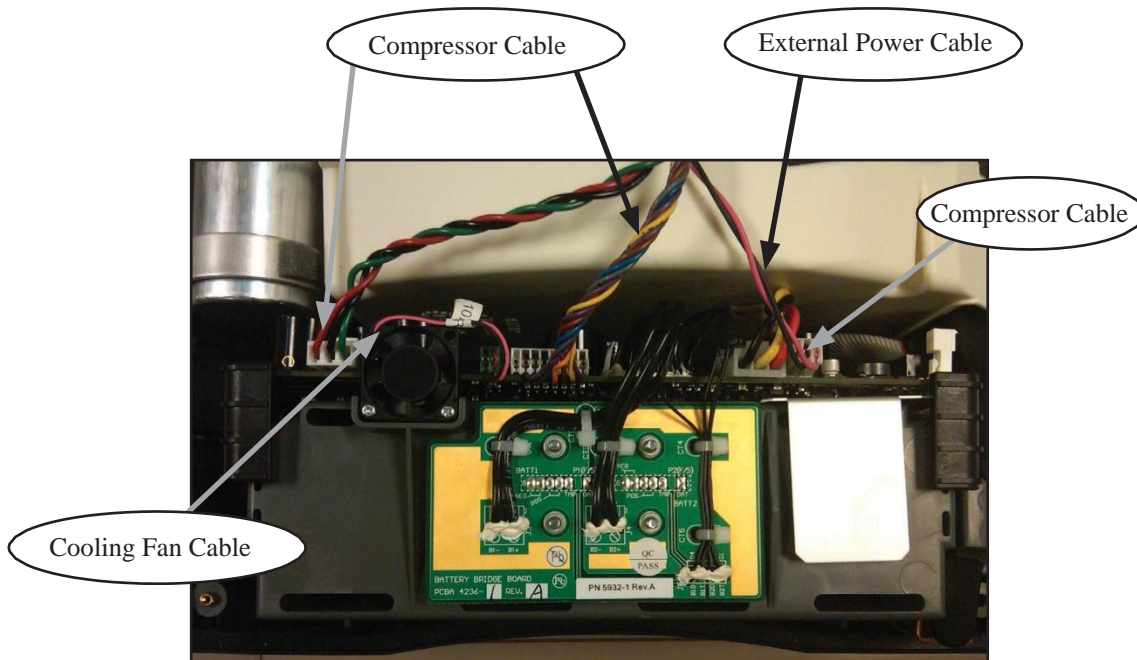


Fig 48: Cable locations

- 1.4 Unscrew the 2 Cooling Fan screws (PN: 6961-21-SEQ) holding the fan in place. Remove the Fan (PN: 1074-SEQ). Set aside for later installation.
- 1.5 Remove the Exhaust tube in Figure 49. Set aside for later installation.

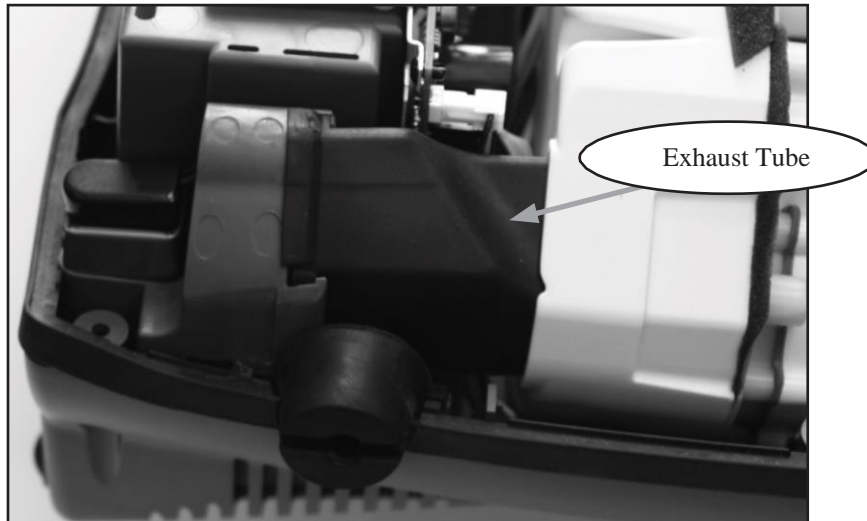


Fig 49: Exhaust Tube

- 1.6 Pull the Power Manager pcb 1”out of the case. Gently push the compressor box away from the Power Manager pcb about 1/8”. Slide the board and the cabling out from under the edge of the compressor for better access. Disconnect the two wire harnesses (9V batt & ATF harness) and the Control board ribbon cable shown in Fig 50. Remove the Power Manager pcb.

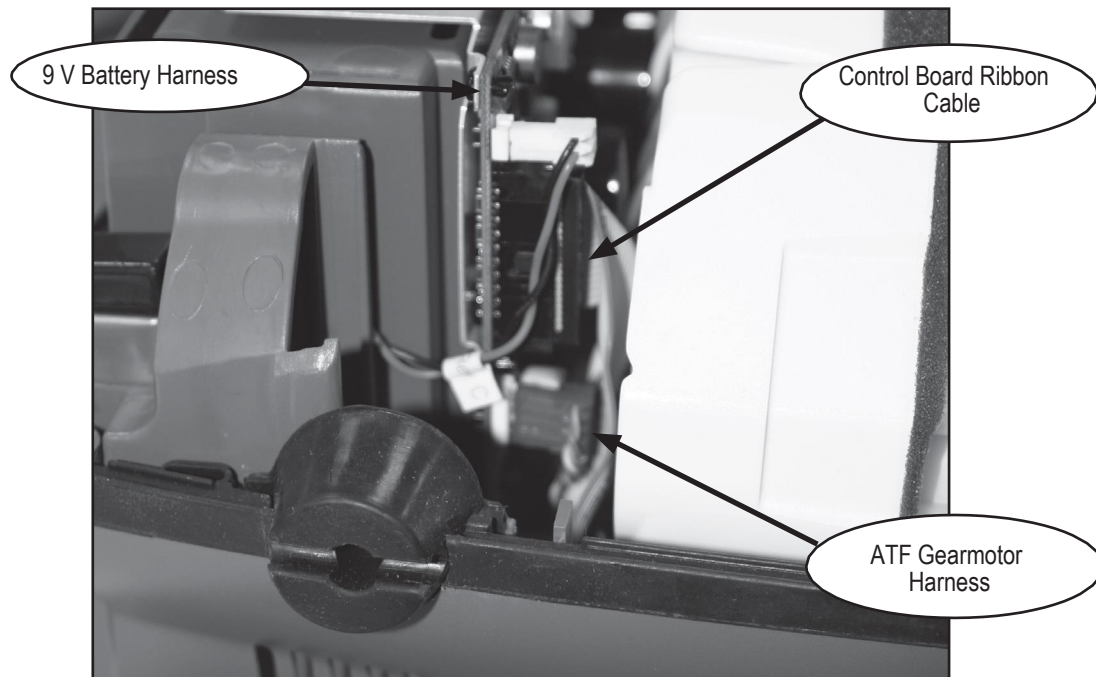


Fig 50: Wire harnesses and control board ribbon

1.7 Unbox the SP5932-4-SEQ and account for all parts (Fig 51).

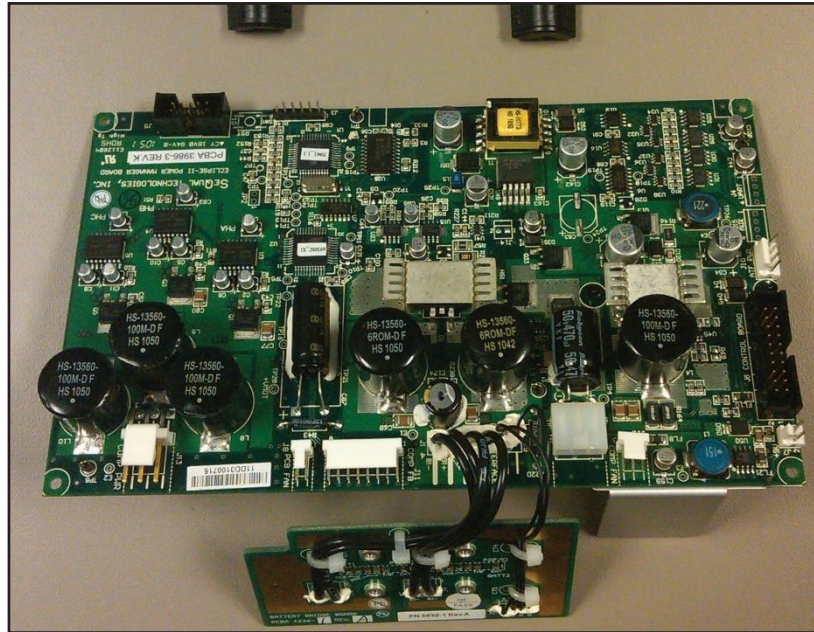


Fig 51: New Power Manager

1.8 Position the Power Manager PCB (PN: SP5932-4-SEQ) 1” out of the case as shown in Fig 52. Gently push the Compressor Box away from the Power Manager pcb by 1/8”. Connect the 2 wire harnesses (Ext Power & ATF harness) and the Control Board Ribbon Cable. **Note:** Route the wiring under the edge of the compressor. Position the Power Manager PCB into the alignment slots on the backcase. Finally connect the 9V battery wiring harness (between the exhaust & battery compartment) and 3 Compressor wiring harnesses to their connectors.

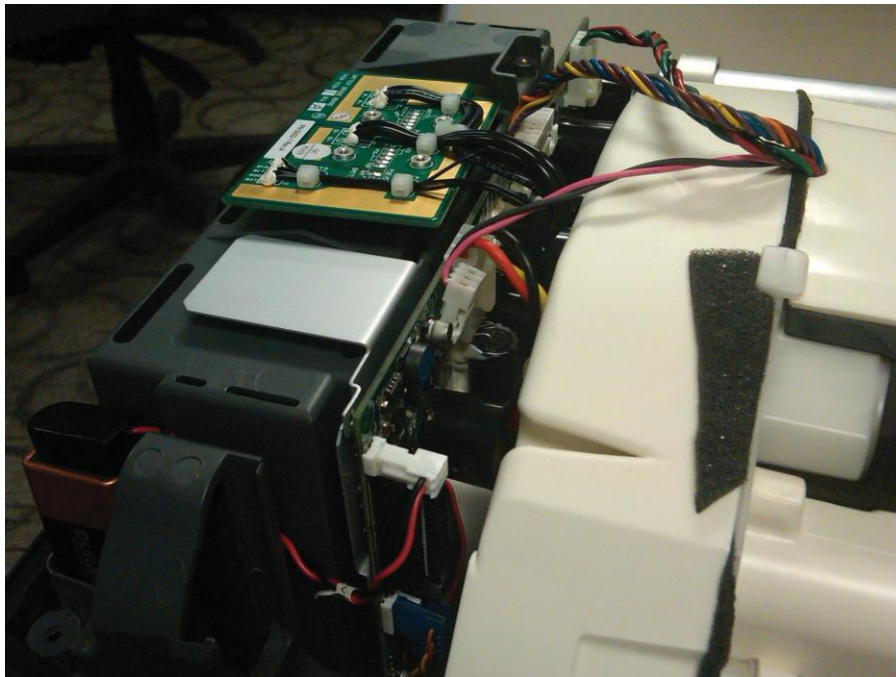


Fig 52: Routing Wires

1.8 Install the Cooling Fan (PN: 1074-SEQ) with the 2 screws (PN: 6961-210-SEQ) and lightly tighten as shown in Fig 53. Apply Loctite 425 thread locker on the tips of the threads before installing.

Note: Ensure the cooling fan is blowing toward the circuit board as indicated by the arrow on the side of the fan.

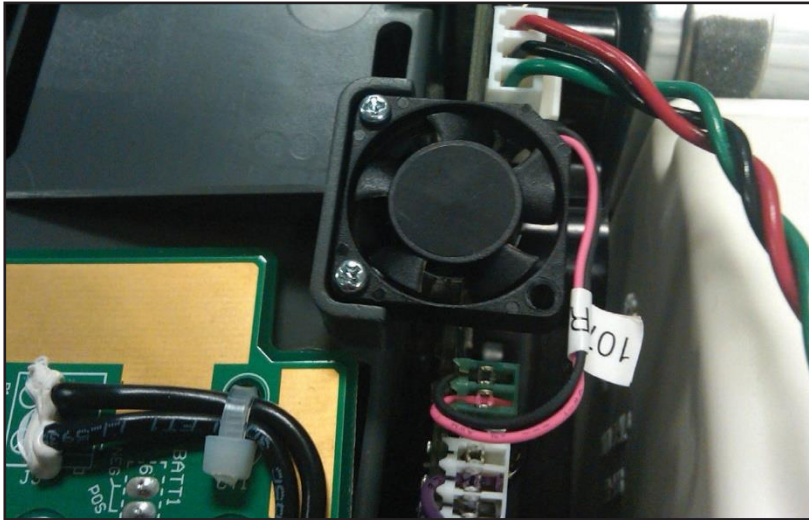


Fig 53: Cooling Fan placement

1.9 Turn the device over and align the BBB with the holes in the case. Screw the 4 screws into the Battery Bridge Board from the Battery compartment side, securing it to the case (snug screws).

1.10 Turn the device back over. Install the 2 clips that come with the power manager board set. **Note:** There is a right and left clip - Large gap is on the right - ensure you get both the metal heat sink and pcb corner in the black clip.

1.11 Install the Unit's front cover according to the "Remove and Replace front cover" section. This holds the Power Manager pcb corner clips in place (no screw required).

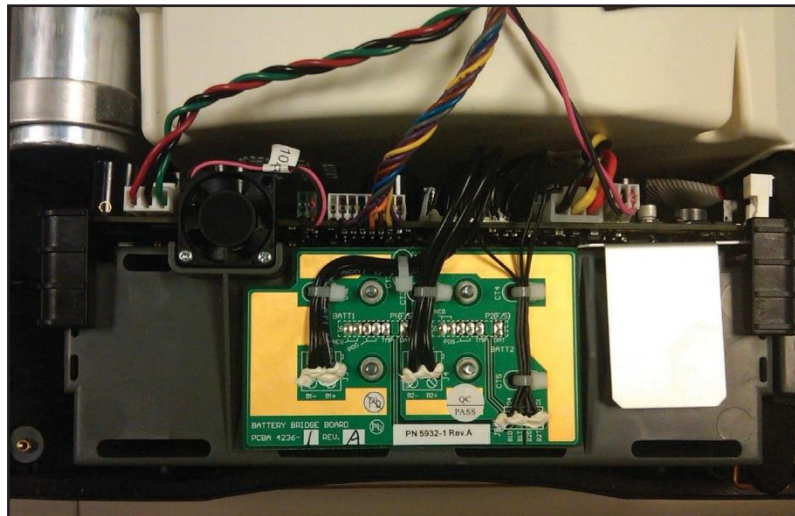


Fig 54: Power Manager installed


Compressor

As with any concentrator, the compressor is a limited-wear component and may require servicing during the lifetime of the device. The point of service will be dependent on factors such as operation time, flow settings and environmental conditions. Service is required when oxygen purity and/or flow rates cannot be maintained.

REMOVE AND REPLACE THE COMPRESSOR BOX

| | |
|--------------|--|
| NOTE: | There are no field serviceable parts inside the Compressor Box. Do not attempt to disassemble or modify the Compressor Box in the field. |
|--------------|--|

1. Remove the Unit Cover as described in the section Remove and Replace the Unit Cover.

| | |
|---|---|
| CAUTION | The Eclipse 5 contains electrostatic sensitive components. Do not open or handle except at a static free workstation. |
|  | |

2. Flip unit over onto a padded ESD safe surface. For 3 Led models use a small flat tip screwdriver to pry open the cover at each pry point, For 2 LED models remove the 2 screws to remove the Case Bottom Cover as shown in Figure 55.



Figure 55: Case Bottom Cover Removal 3 LED model left photo, 2 LED model right photo

3. Disconnect the 3 wire harnesses shown in Figure 56.

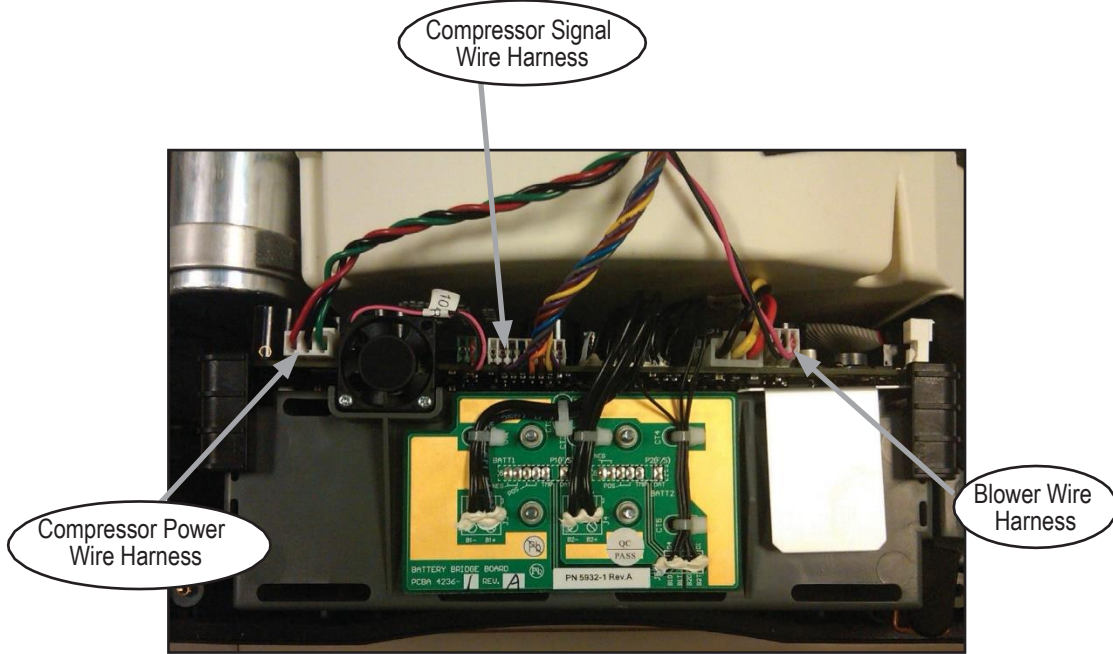


Figure 56: Compressor Box electrical connections.

4. Remove the Exhaust Tube as shown in Figure 57.

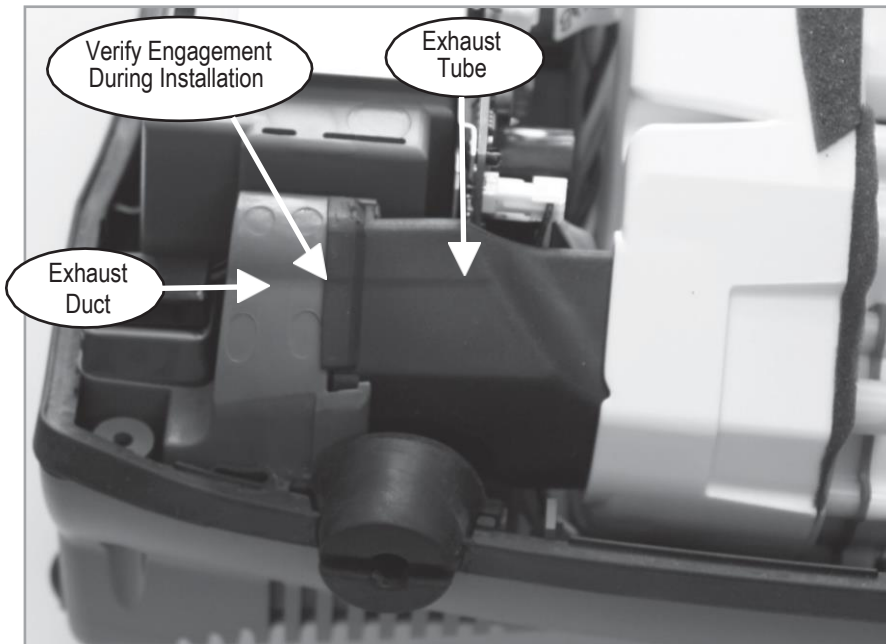



Figure 57: Exhaust Tube Removal.

5. Cut the three cable ties shown in Figure 58. Disconnect the two braided hoses from the pressure and vacuum ports of the ATF. Cap the three ATF module ports using tight fitting vinyl caps or vinyl electrical tape.

| | |
|---|--|
| CAUTION | Once the braided hoses are disconnected from the ATF Module the ATF Module is exposed to the atmosphere. Cap the ATF Module ports immediately in order to minimize exposure to debris and humidity which may result in ATF Module damage. |
|  | |

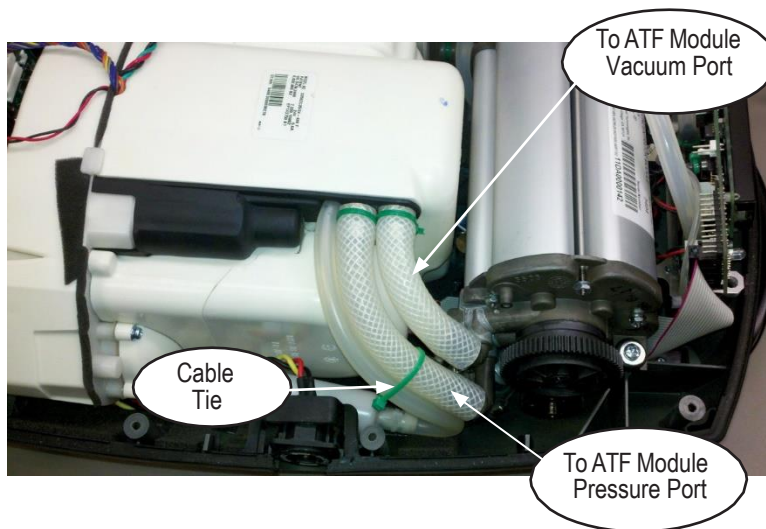


Figure 58: Removal of Compressor Pressure and Vacuum Hoses from ATF Module.

6. Turn the unit over onto a padded ESD safe surface and remove the 4 screws (M4x16 Pan Head Machine Screw, PN 6961-420-SEQ) and washers (M4 Flat Fender Washer, PN 3568-SEQ) shown in Figure 59.



Figure 59: Remove Compressor Box screws.

| | |
|-------|--|
| NOTE: | There are no field serviceable parts inside the Compressor Box. Do not attempt to disassemble or modify the Compressor Box in the field. |
|-------|--|

7. Remove the Compressor Box.
8. To install the Compressor Box, lay the new Compressor Box in the unit. Turn over the unit.
9. Position the Compressor Box into the Bottom Case with the compressor box screw holes aligned with the 4 brass eyelets. Screw in the 4 screws and 4 washers as shown in Figure 59. Apply small amount of Loctite 425 on the threaded tips of the screw before installing.
10. Install the braided tubes into the ATF pressure and vacuum ports as shown on Figure 58 on previous page. Secure joints with cable ties.
11. Use a cable tie to secure the silicone tube to the braid tube to ensure that there is NO kinking on the bend as shown on Figure 58 on previous page. Hand tighten the cable tie. Inspect the tubing to ensure the tubing is not kinked.
12. Hold onto the Compressor Box and lift the Bottom Case into a standing position. Insert the Exhaust Tube into the slot of the Exhaust Duct as shown on Figure 57. Ensure that it is secure without any gaps.
13. Plug the 3 harnesses into the Power Manager PCB as shown on Figure 56.
14. Install the Case Bottom Cover as shown in Figure 55.
15. Install the Unit Cover as described in the section Remove and Replace the Unit Cover as outlined on page 39.
16. EDAT may be utilized to record Eclipse 5 device status and dates of service.

MAINTENANCE AND REPLACEMENT PARTS

Preventative Maintenance Parts

| Description | CAIRE Inc. Part Number |
|---|------------------------|
| Preventive Maintenance Kit (includes * items) | 5022-SEQ |
| * Air Inlet Filter | 7028-SEQ |
| * Compressor Intake Filter | 8069-SEQ |
| * HEPA Filter (Old /New) | 6986-SEQ / 9765-SEQ |
| * 9V Battery | 8098-SEQ |
| * Wire Ties (Qty 10) | 5268-SEQ |
| EDAT (Service Tool) | 5535-SEQ |

Replacement Parts List

| Description | CAIRE Inc. Part Number |
|--|--|
| AC Power Supply—3 LED | 5941-SEQ |
| AC Power Supply—2 LED | 20852326S (with IEC type A cord) 20852325S (with IEC type C cord) 20852324S (with IEC type G cord) |
| ATF Module Assembly, Eclipse 5 | 20626702 |
| Cable harness, SPI/ I2C—3 LED only | 8076-SEQ |
| Carton Assembly, Eclipse 5 Oxygen System | SP3581-SEQ |
| Case Bottom Cover—3 LED only | 20623857 |
| Case Bottom Subassembly, Eclipse 5—3 LED only | SP20623837 |
| Case Top Subassembly, Eclipse 5—3 LED only | SP20623840 |
| Front Case—2 LED | 21177237 |
| Rear Case—2 LED | 21126775 |
| Compressor Box Assembly, Universal | SP5999-SEQ |
| Control System PCBA, Eclipse 5—3 LED only | SP4043-9-SEQ |
| DC Power Supply | 5942-SEQ |
| Foot, bottom | 6956-SEQ |
| Handle | 6963-SEQ |
| Inlet Filter | 7028-SEQ |
| Membrane Panel Overlay, Eclipse 5—3 LED | SP20618461 |
| Membrane Panel—2 LED | 21072187 |
| Nut, Outlet | 2777-SEQ |
| Outlet Assembly, Oxygen | 3922-SEQ |
| Power Manager PCBA, Eclipse 5 (Not Field Replaceable)—3 LED only | SP5932-4-SEQ |
| CB PCBA—2 LED | 21122262 |
| Power Manager Assembly—2 LED | 5932-2-SEQ |
| Power Cartridge | 7082-SEQ |
| Product Tank Assembly | SP4378-SEQ |
| Rubber Gasket (Channel Seal)—3 LED only | 4106-2-SEQ |
| Gasket—2 LED | 21108146 |
| Screw, M2x10 Pan Head Machine (Cooling fan) | 6961-210-SEQ |
| Screw, M3x10 Plastite (CS pcb, Product Tank, 9V Batt harness) | 6950-310-SEQ |
| Screw, M3x12 Pan Head SEM (Top to Bottom case, BBB PCB) | 6974-312-SEQ |
| Screw, M4x16 Pan Head Machine (ATF to Bottom case) | 6961-416-SEQ |
| Screw, M4x16 Pan Head Machine (Compressor to Bottom Case) | 6961-420-SEQ |
| Tubing, Silicone, 3/16"ID | SP6981-SEQ |
| Tubing, Silicone, 2mm ID | SP4101-SEQ |
| Tubing, Braided, 5/16"ID | SP3534-SEQ |
| Washer, M3 Flat | 6985-03-SEQ |
| Washer, M4 Flat | 6985-04-SEQ |
| Washer, M4 Flat Fender | 3568-SEQ |
| Wire harness, 9V | 1076-SEQ |
| Wire Harness, Service Port | 7012-SEQ |
| Wire Harness, External Power, Eclipse 5 | 4063-SEQ |
| Kit, Preventative Maintenance | 5022-SEQ |

OPTIONAL ACCESSORIES

Visit us at www.sequal.com for more information about optional accessories. There are many different types of oxygen tubing, cannula, and humidifiers. The following items are recommended by CAIRE Inc. for use with the Eclipse 5.

Salter Labs[®] Humidifier, Part Number 7600, or equivalent: If your physician has prescribed an optional humidifier, follow the manufacturer's instructions for use. Attach the humidifier to the oxygen outlet port of the Eclipse 5. Use of optional humidifiers not recommended for the Eclipse 5 may impair performance of the device and may void the warranty.

DO NOT use a humidifier in the Pulse Flow Mode. The Eclipse 5 will not detect inspiratory effort. The device will alarm and default to the Continuous Flow Mode for continuing operation after 15 seconds.

CAIRE Humidifier Adapter – Part Number 7116-SEQ: If your physician has prescribed an optional humidifier, you may need to use the CAIRE Humidifier Adapter. Follow the instructions for use. Attach the Humidifier Adapter to the oxygen outlet port of the Eclipse 5 and then to the humidifier. Attach the cannula, or oxygen tubing to the humidifier outlet.

Salter Labs Oxygen Supply Tubing, Part Number Series 2000, or equivalent: The internal diameter should be no less than 3/16" (0.48 cm). Connect the oxygen tubing to the outlet port of the humidifier, or directly to the oxygen outlet port of the Eclipse 5 if you do not use a humidifier. Connect the other end of the tube to the nasal cannula, if oxygen supply tubing is not already attached to the cannula. Tubing not specified for use with this Eclipse 5 may impair the performance of the device.

Salter Labs Oxygen Cannula, Part Number 1600 Series, or equivalent: Your physician will have prescribed a cannula to deliver oxygen. In most cases they are already attached to the oxygen tubing. If not, follow the instructions included with the cannula to attach it to the oxygen tubing. Use of an oxygen cannula not specified for use with this Eclipse 5 may impair the performance of the device.

CAIRE INC. CUSTOMER SERVICE CONTACT INFORMATION

If you need any additional assistance, contact CAIRE Inc:



By mail:

CAIRE, Inc.
2200 Airport Industrial Drive, Suite
500 Ball Ground, GA 30107 USA

By telephone: 800.482.2473

www.CAIREmedical.com

AUTHORIZED EUROPEAN UNION REPRESENTATIVE:



Medical Product Services GmbH
Borngasse 20
35619 Braunfels, Germany

www.CAIREmedical.com

SeQual[®], ATF[®] and Eclipse 5[®] are registered trademarks of CAIRE Inc.
PRO2 Check EliteTM is a trademark of Salter Labs Inc.
Lysol[®] is a registered trademark of Reckitt Benckiser, UK.
Loctite[®] is a registered trademark of Loctite Corporation, USA.
HydroPure[®] and Hydroklean[®] are registered trademark of Contec, Inc.



0459
Copyright © 2018 CAIRE Inc. CAIRE Inc. reserves the right to discontinue its products, or change the prices, materials, equipment, quality, descriptions, specifications and/or processes to its products at any time without prior notice and with no further obligation or consequence. All rights not expressly stated herein are reserved by us, as applicable.